





US 20200124596A1

(19) **United States**(12) **Patent Application Publication**
SIM(10) **Pub. No.: US 2020/0124596 A1**(43) **Pub. Date: Apr. 23, 2020**(54) **BIOSENSOR FOR DIAGNOSING
ALZHEIMER'S DISEASE USING RAYLEIGH
SCATTERING AND COLORIMETRIC ASSAY
OF GOLD NANOPARTICLE AND
MULTI-DETECTION METHOD USING THE
BIOSENSOR****G01N 33/68** (2006.01)**G01N 21/25** (2006.01)(52) **U.S. Cl.**CPC . **G01N 33/54346** (2013.01); **G01N 33/54393**
(2013.01); **G01N 33/531** (2013.01); **B82Y 5/00**
(2013.01); **G01N 21/25** (2013.01); **G01N**
2800/2821 (2013.01); **G01N 33/6896**
(2013.01)(71) Applicant: **PHARMAWORKS CO., LTD.**, Seoul
(KR)(72) Inventor: **SangJun SIM**, Seoul (KR)(73) Assignee: **PHARMAWORKS CO., LTD.**, Seoul
(KR)(21) Appl. No.: **16/686,610**(22) Filed: **Nov. 18, 2019****Related U.S. Application Data**(63) Continuation-in-part of application No. 15/971,688,
filed on May 4, 2018, now abandoned.**Publication Classification**(51) **Int. Cl.****G01N 33/543** (2006.01)**G01N 33/531** (2006.01)(57) **ABSTRACT**


The present invention relates to a nanoplasmonic sensor based on gold nanoparticle to which an antibody or an aptamer binds, the antibody or the aptamer recognizing A β 1-40, A β 1-42, and τ protein, which are Alzheimer's disease onset markers that are present in blood, and a multi-detection method of Alzheimer's disease using Rayleigh scattering phenomenon and colorimetric assay of the sensor. The present invention has advantages in that it is possible to perform simultaneous multiple detect with respect to various onset markers by using a simple diagnosis method using blood, and sensitivity of diagnosis is improved by using a chaotropic solvent.

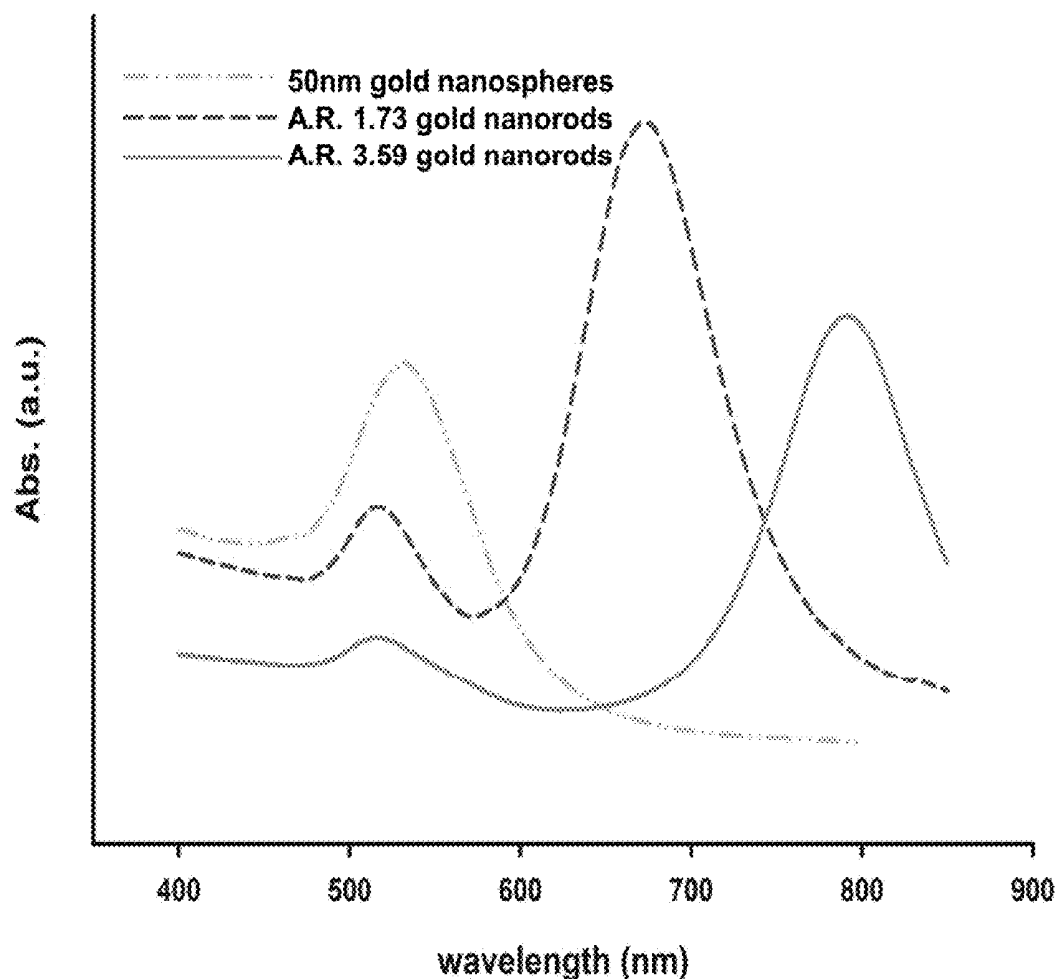

【Figure 1】

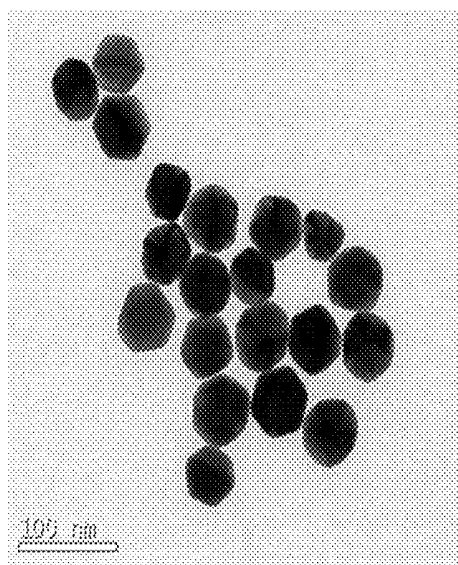

【Figure 2】

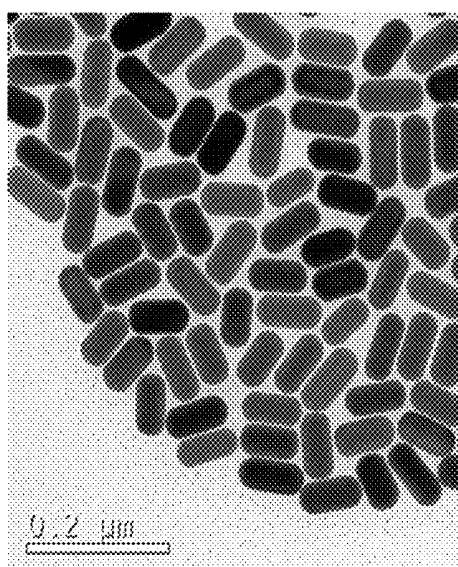

【Figure 3】

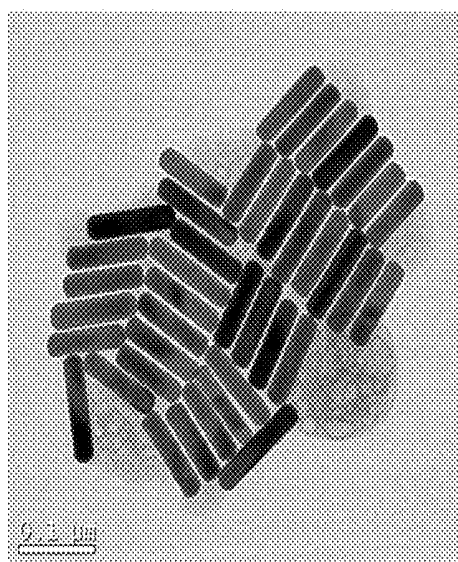


FIG. 4

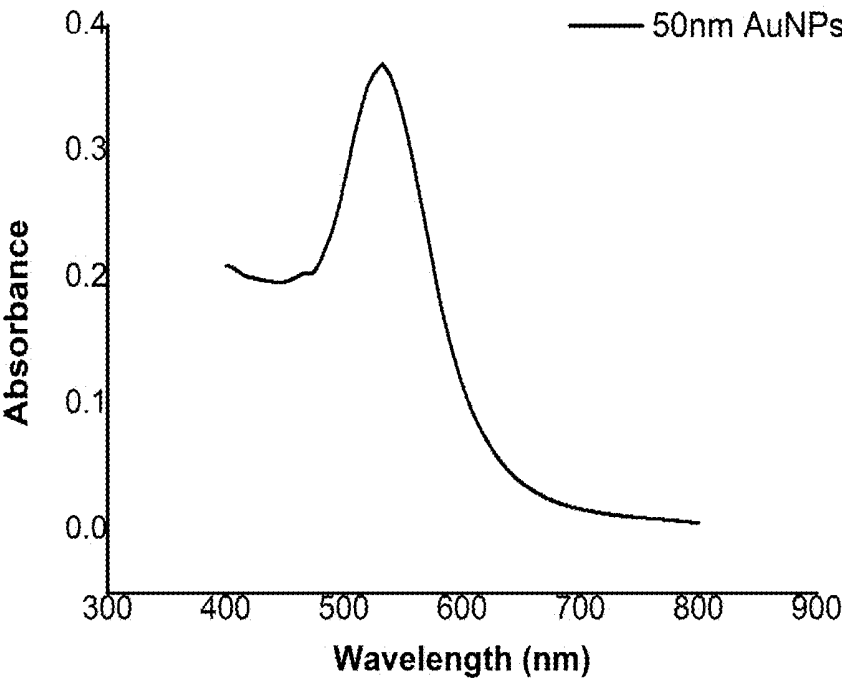


FIG. 5



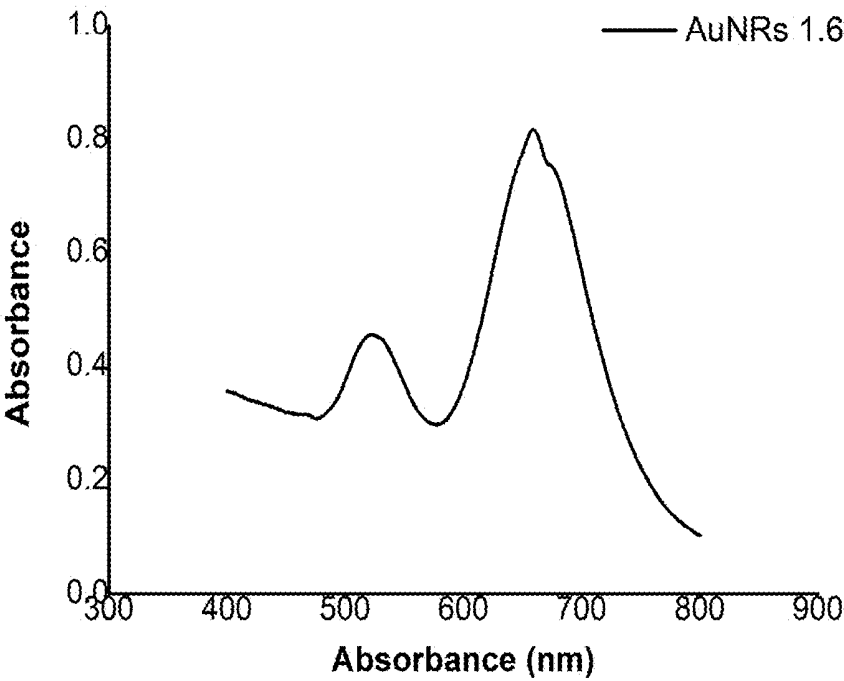



FIG. 6

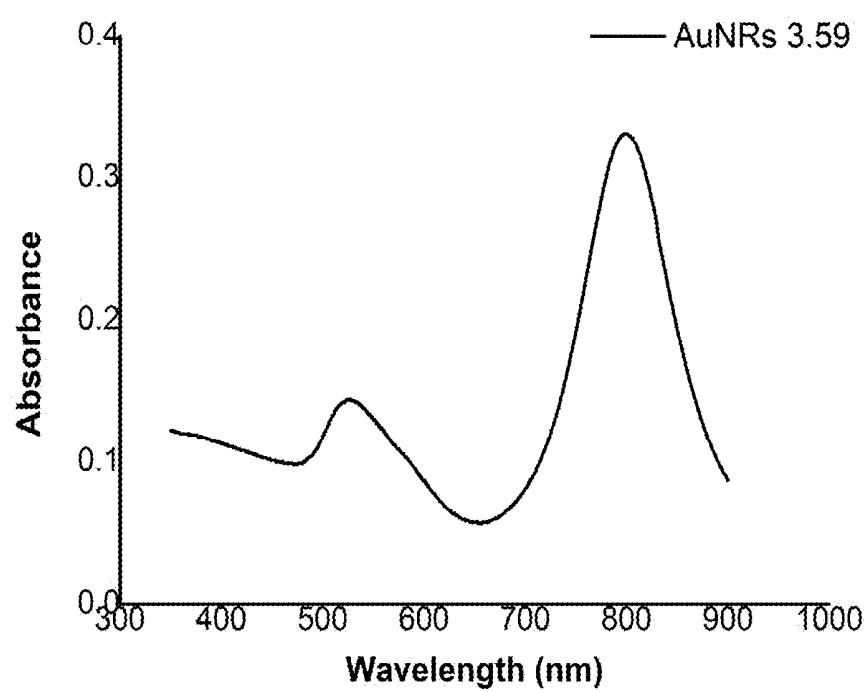


【Figure 7】

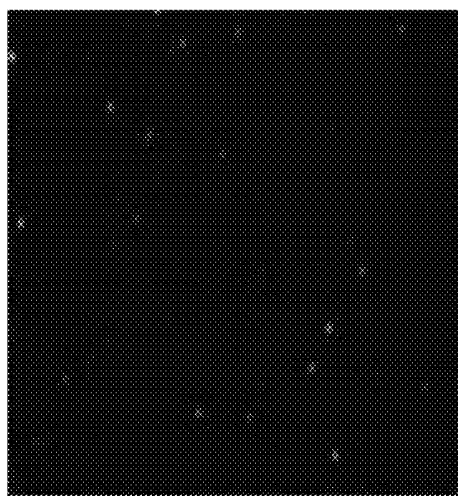


【Figure 8】

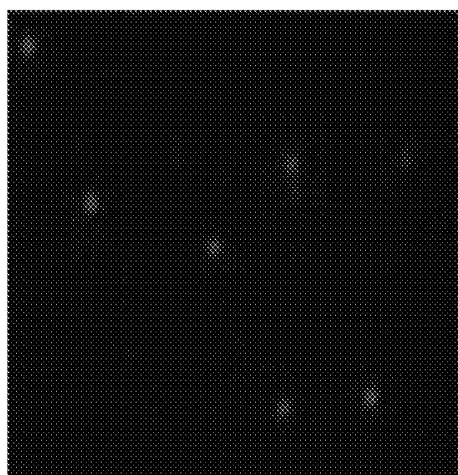


【Figure 9】

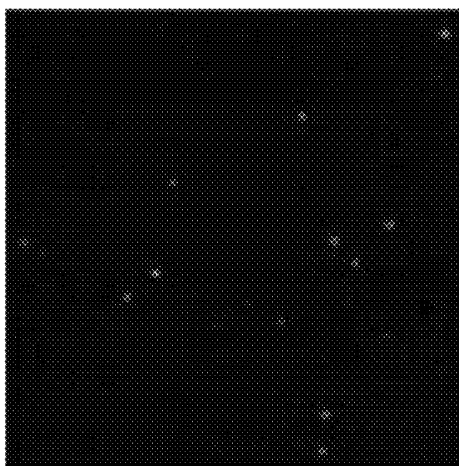


【Figure 10】

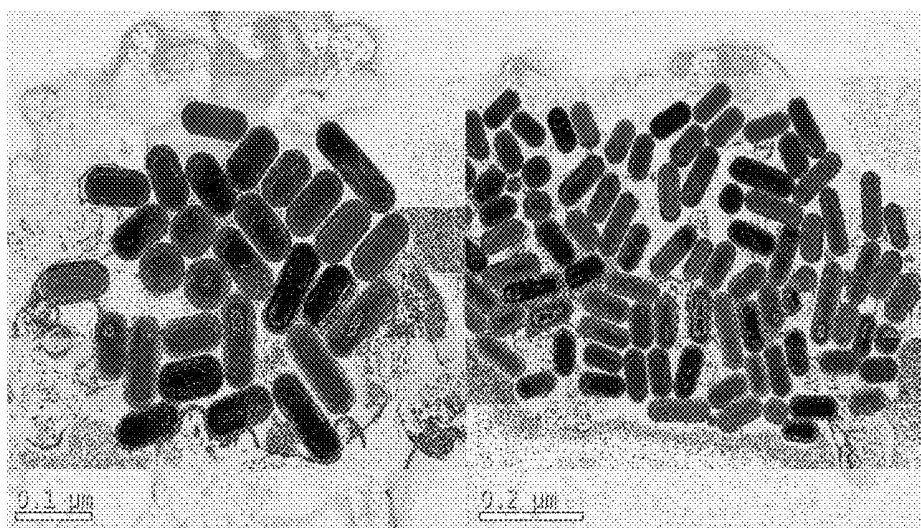


【Figure 11】

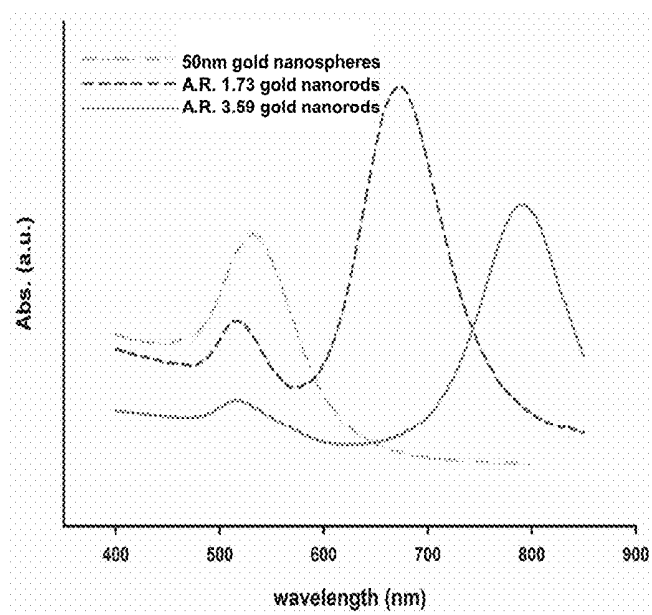

【Figure 12】

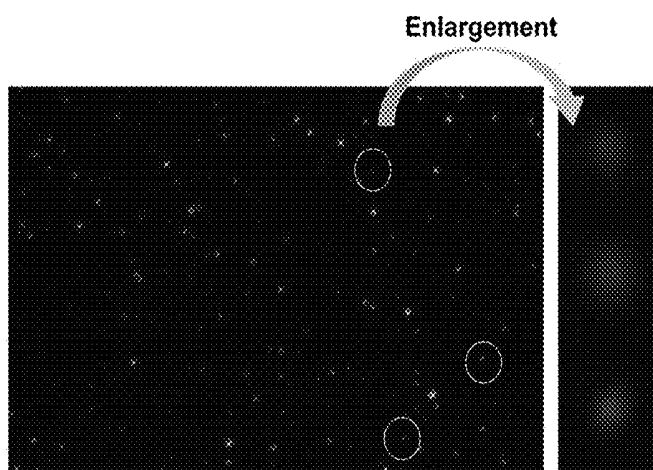

【Figure 13】

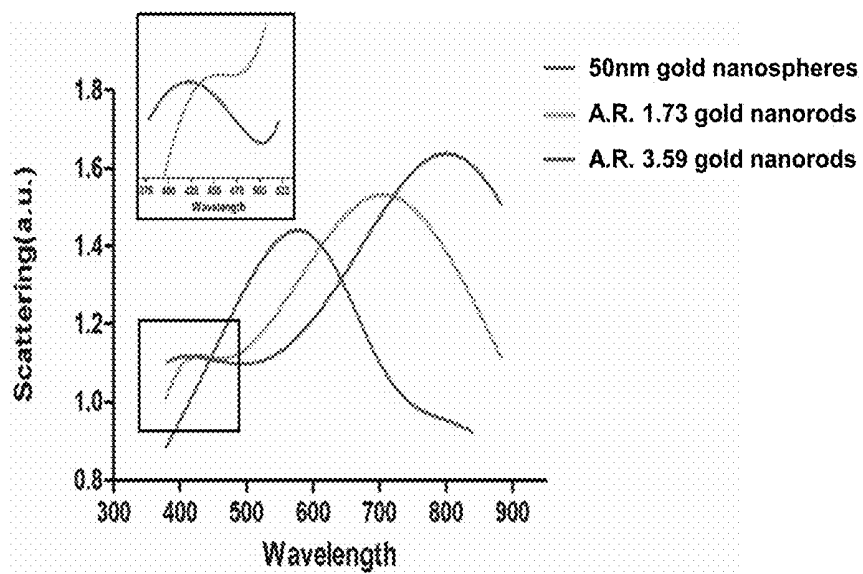

【Figure 14】


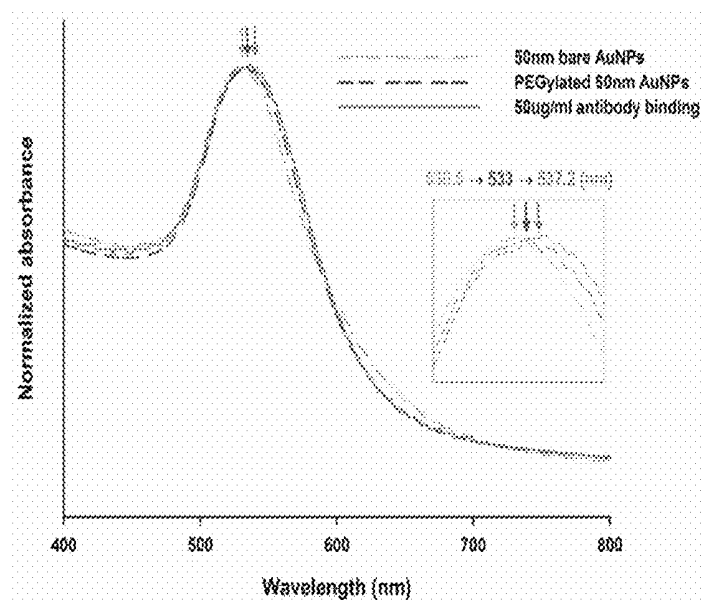


FIG. 15

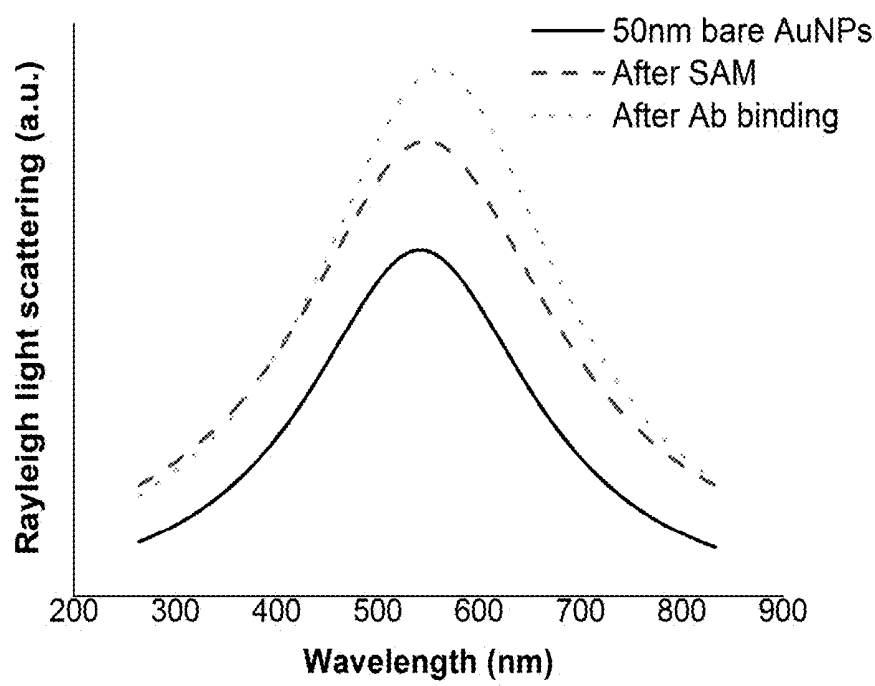

【Figure 16】

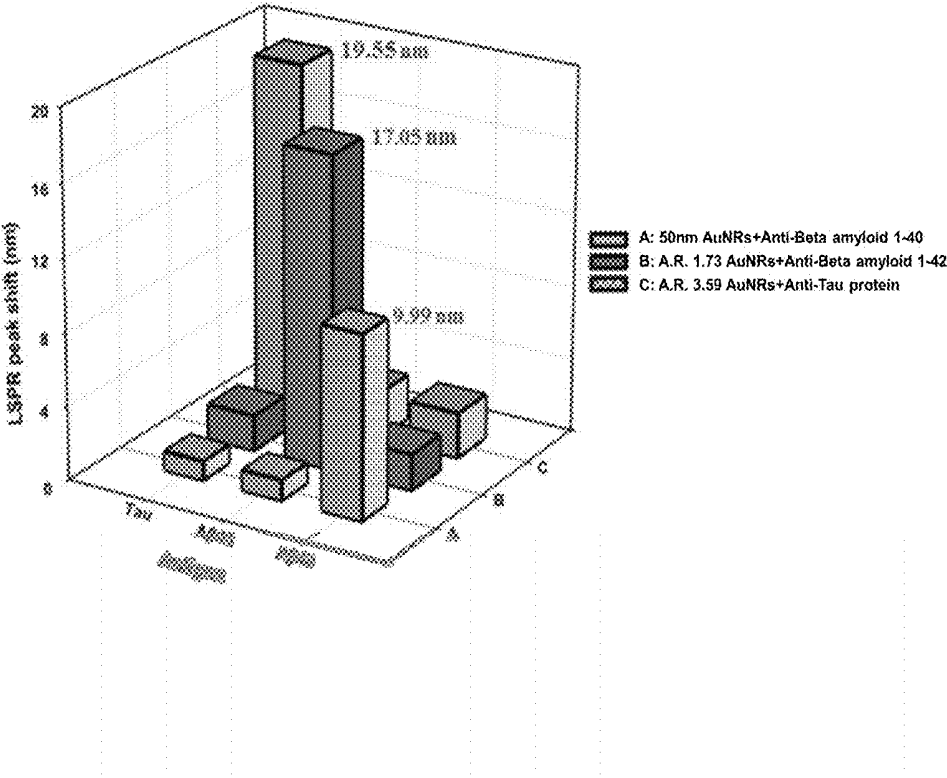


FIG. 17A

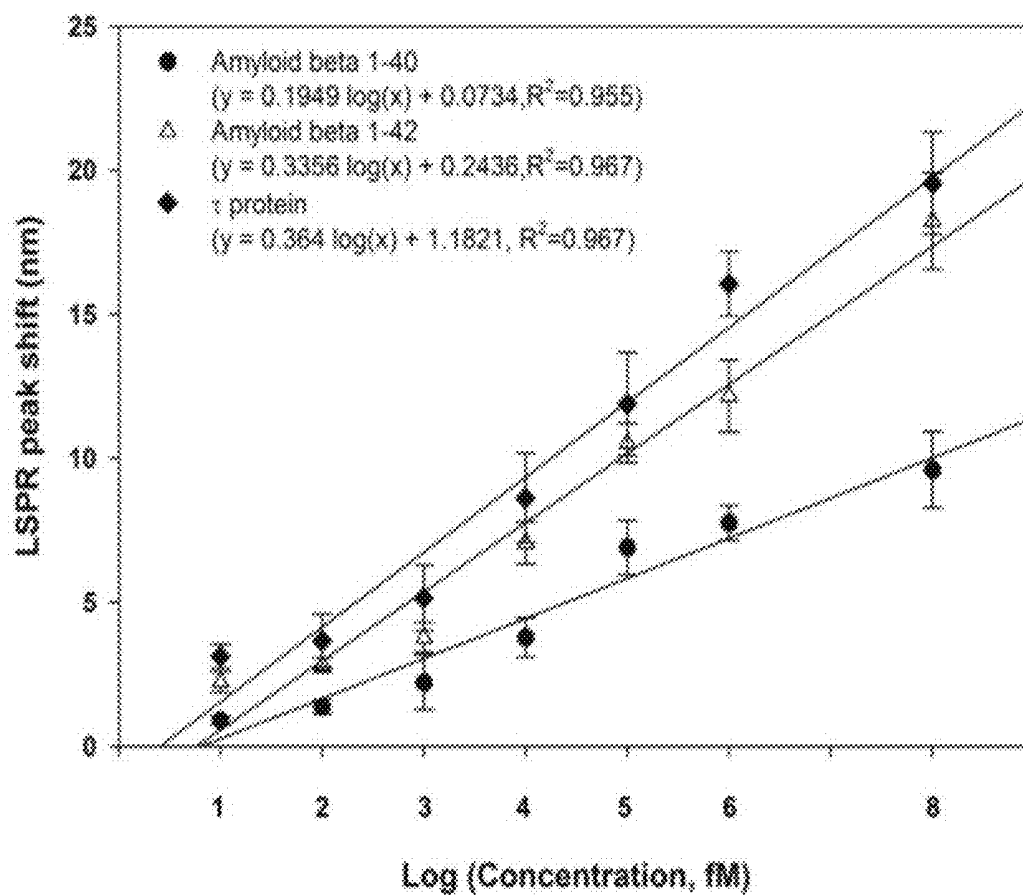


FIG. 17B


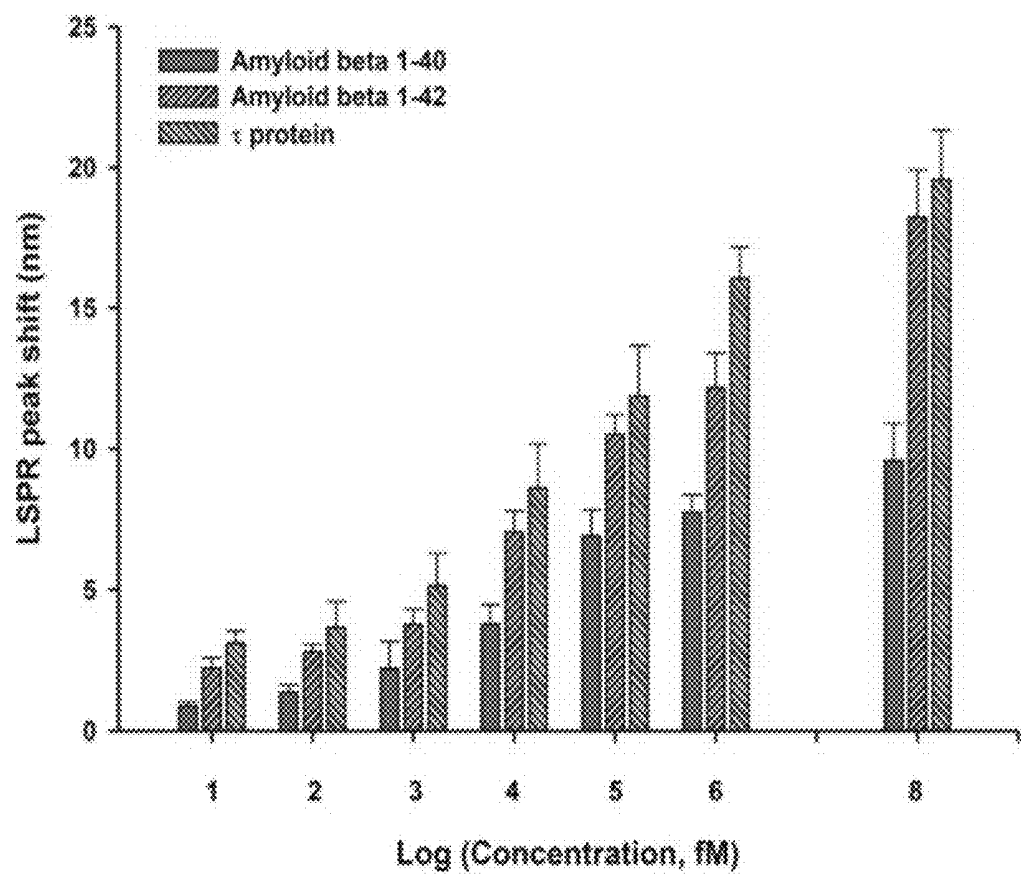


FIG. 18

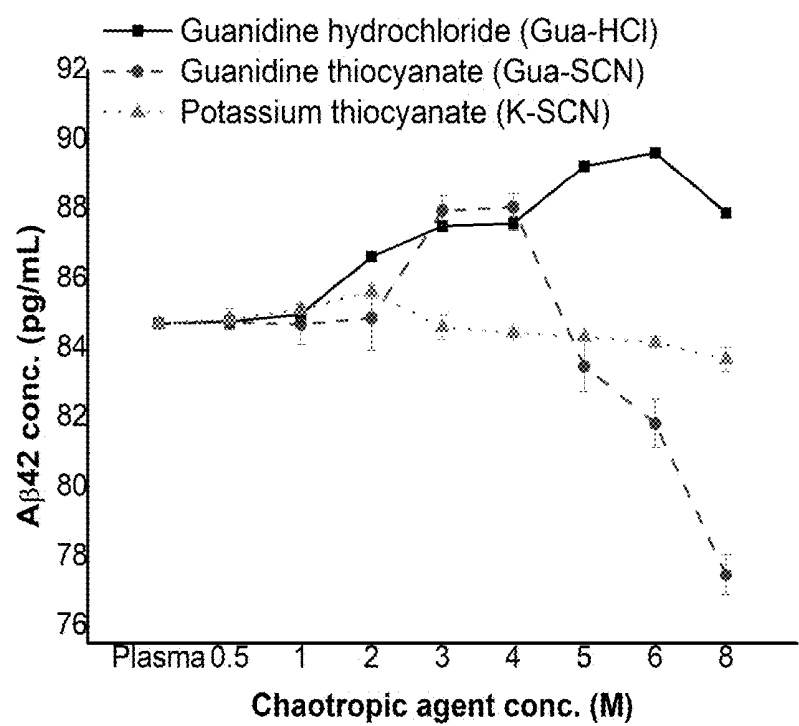

【Figure 19】

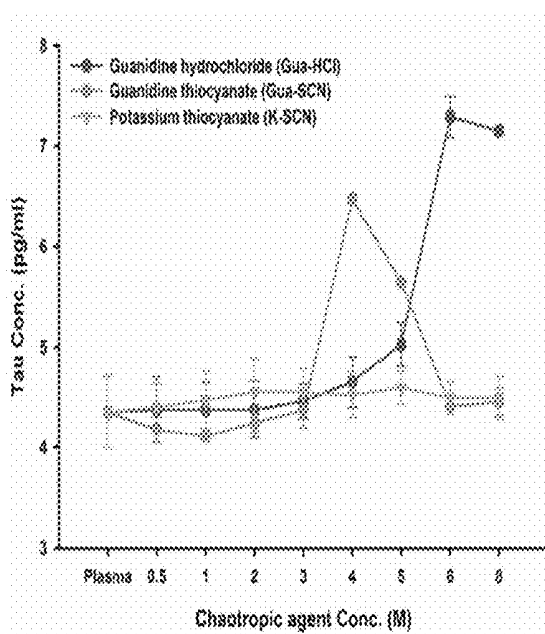


FIG. 20



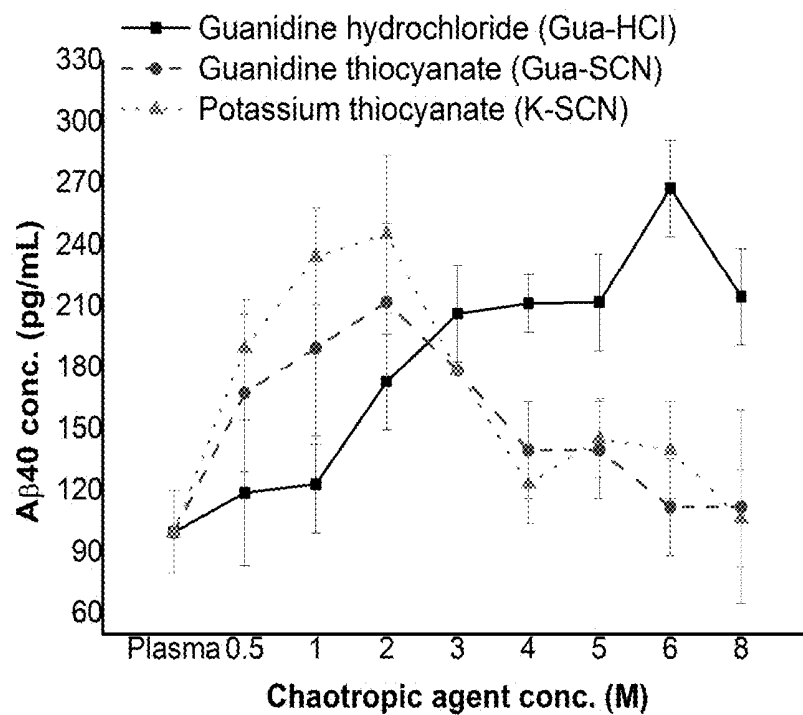


FIG. 21B

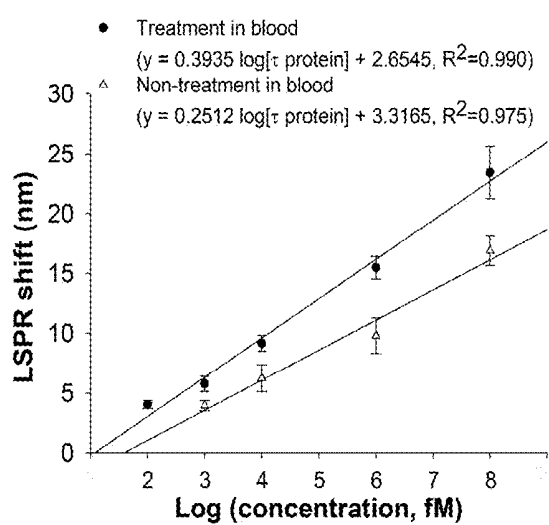

【Figure 22】

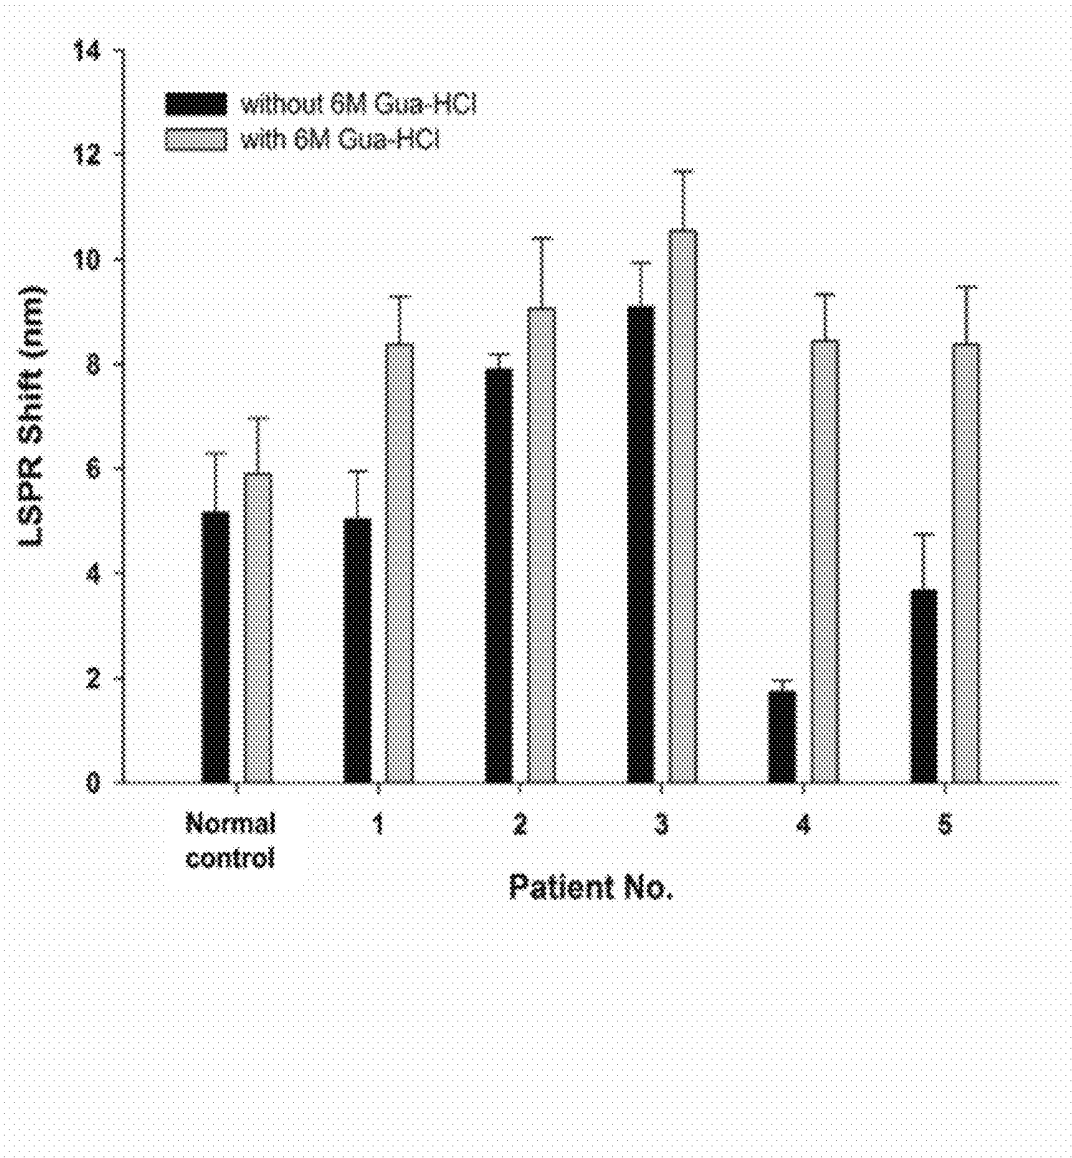

**BIOSENSOR FOR DIAGNOSING
ALZHEIMER'S DISEASE USING RAYLEIGH
SCATTERING AND COLORIMETRIC ASSAY
OF GOLD NANOPARTICLE AND
MULTI-DETECTION METHOD USING THE
BIOSENSOR**

**CROSS-REFERENCE TO RELATED
APPLICATIONS**

[0001] This application is a continuation in part of U.S. patent application Ser. No. 15/971,688 filed on May 4, 2018, the entire disclosure of which is incorporated herein by reference for all purposes.

TECHNICAL FIELD

[0002] The present invention relates to a biosensor for diagnosing Alzheimer's disease using Rayleigh scattering and colorimetric assay of a gold nanoparticle and a multi-detection method using the biosensor, and more particularly, to a nanoplasmonic sensor recognizing A β 1-40, A β 1-42, and τ protein, which are Alzheimer's disease onset markers that are present in blood, and a multi-detection method of Alzheimer's disease using the sensor.

BACKGROUND ART

[0003] Alzheimer's disease has histological features of amyloid plaque and neurofibrillar tangle at the hippocampus and cortex, and is a degenerative disease that weakens social function of a patient by exacerbating cognitive disorder affecting the patient's memory. Alzheimer's disease is a type of disease that has slow a disease progression rate, but the disease progresses above a certain level is not able to be remissible, and thus early diagnosis is very important. To date, diagnostic methods include brain imaging, cognitive testing, and examination through cerebrospinal fluid, etc. However, these methods are applicable only after symptoms of Alzheimer's disease are manifested, which is insufficient for early diagnosis. In addition, a lot of economic cost for diagnosis is required, and it is accompanied by an operative method, and thus the risk is very high. Therefore, it is important to develop a simple method for early diagnosis of Alzheimer's disease, and thus, there is an urgent need to develop a highly sensitive diagnostic method for detecting a trace amount of onset biomarker present in blood.

[0004] Currently, a material that is considered as the most important indicator as a causative agent in pathogenesis of Alzheimer's disease includes A β 1-40, A β 1-42 peptide, and τ protein, etc.

[0005] The beta-amyloid peptide is produced by cleaving an amyloid precursor protein by beta-secretase and gamma-secretase. Thus, as activity of these enzymes increases, the production of beta-amyloid peptide increases, which is closely related to Alzheimer's disease. However, if the alpha-secretase which cleaves an intermediate region of the beta-amyloid peptide increases its activity, the production of beta-amyloid peptide rather decreases. Alpha-secretase predominates in normal subjects and prevents amyloid beta cleavage by beta-secretase. When these beta-amyloid peptides accumulate in the brain, large amounts of reactive oxygen are produced, causing oxidative damage and causing death of nerve cells. In addition, beta-amyloid peptide causes excessive accumulation of intracellular calcium, causing cell death due to excitotoxicity. The death of nerve

cells due to the beta-amyloid peptides, particularly, cell death in hippocampus, a region associated with memory, induces memory loss, which is a typical symptom of dementia. A major plaque component of beta-amyloid produced by sequential cleavage by the secretase is known as isoform of A β 1-42 peptide involved in formation of neurotoxic oligomer and plaque formation in an onset mechanism of Alzheimer's disease.

[0006] Recently, it has been reported that in addition to beta-amyloid, τ protein has an abnormal structure and forms an inclusion body, which causes degenerative brain disease. It is known that the τ protein is necessary to stabilize microtubules like a connecting steel of a railroad. As the τ protein accumulates excessively, the microtubules collapse and a network of normal nerve cells breaks down. A cause of accumulation of the τ protein is that phosphorus is excessively attached to the τ protein to form a polymer due to phosphorylation, and a disease caused by accumulation of the τ protein and aggregation of nerve cells is called Tophathy and has been indicated as a cause of various degenerative brain diseases.

[0007] Meanwhile, recently, biosensor technology has focused on development of non-labeling measurement technology that does not use a labeling material, and typically includes a method of using a surface plasmon resonance phenomenon occurring on a metal surface (R. Q. DUAN et al., *Neoplasma*, 59(3):348, 2012; Wei Zhou et al., *International Journal of Nanomedicine*, 6:381, 2011), a method of measuring a change in refractive index of light due to bending phenomenon of a cantilever which is a three-dimensional microstructure (Balle, M K. et al., *Ultramicroscopy*, 82; 1, 2000), a method of measuring a change in resonance frequency of crystals according to a change in mass of biomolecules (Marx, K A., *Biomacromolecules*, 4; 1099, 2003), a method of measuring an electric field effects based on semiconductor process (Yuqing, M. et al., *Bio-technol. Adv.*, 21; 527, 2003), and an electrochemical measurement method (Hanahan, G. et al., *J. Environ. Monit.*, 6; 657, 2004; Sang Hee Han et al., *Analytica Chimica Acta*, 665:79, 2010), etc.

[0008] Among them, the localized surface plasmon resonance (LSPR) method is able to quantitatively detect a reaction without complicated pre-purification and labeling processes, and thus it has been used in a number of studies on interaction between biomolecules immobilized on a surface. In the LSPR method, when light having various wavelengths is irradiated to a material having a localized surface such as a metal nanoparticle, unlike a bulk metal, polarization is generated on a surface of the metal nanoparticle, and a peculiar characteristic that intensity of the electric field is increased is shown. LSPR optical property is sensitive to a change in dielectric constant (refractive index) generated near the nanoparticle. This change in dielectric constant (refractive index) may be used to detect adsorption between biomolecules. For the past several decades, various biomolecule interaction analyses have been performed based on the optical properties of the LSPR to measure biomaterial concentration, thickness, and binding reaction rate data for a particular biochemical analyte, including antigen/antibody, ligand/receptor, protein/protein reaction, and DNA hybridization.

[0009] Therefore, the present inventors have made intensive efforts to develop a novel multiple detection platform capable of early diagnosis of Alzheimer's disease, and as a

result, confirmed that A β 1-40, A β 1-42, and τ protein, which are three markers of Alzheimer's disease onset that are present in blood, could be detected using a nanoplasmonic sensor, and completed the present invention.

RELATED ART DOCUMENT

(Patent Document 1) Korean Patent No. 10-1003124

DISCLOSURE

Technical Problem

[0010] An object of the present invention is to provide a method for diagnosing Alzheimer's disease using Rayleigh scattering and colorimetric assay of a plasmonic sensor based on a gold nanoparticle to which an antibody is immobilized, and a biosensor for diagnosing Alzheimer's disease.

Technical Solution

[0011] In order to achieve the foregoing objects, the present invention provides a method for diagnosing Alzheimer's disease comprising (A) contacting a sample separated from a specimen with a plasmonic sensor based on a gold nanoparticle to which an antibody or an aptamer specific to a target protein of which expression is specifically increased or decreased in Alzheimer's patient is immobilized, thereby inducing a binding between the target protein and the antibody or the aptamer; (B) measuring light scattering spectrum according to the binding; and (C) determining whether or not Alzheimer's disease occurs through analysis of maximum wavelength mobility (λ_{max}) obtained from the spectrum.

[0012] The present invention also provides a biosensor for detecting Alzheimer's disease in which an antibody or an aptamer of at least one target protein selected from the group consisting of A β 1-40 peptide, A β 1-42 peptide, and τ protein is immobilized to a gold nanoparticle.

DESCRIPTION OF DRAWINGS

[0013] FIG. 1 shows an HR-TEM image of a 50 nm-sized circular gold nanoparticle produced in Example 1-1.

[0014] FIG. 2 shows an HR-TEM image of a rod-shaped gold nanoparticle having an aspect ratio of 1.73 and produced in Example 1-2.

[0015] FIG. 3 shows an HR-TEM image of a rod-shaped gold nanoparticle having an aspect ratio of 3.59 and produced in Example 1-3.

[0016] FIG. 4 shows UV-Vis spectrum of the 50 nm-sized circular gold nanoparticle produced in Example 1-1.

[0017] FIG. 5 shows UV-Vis spectrum of the rod-shaped gold nanoparticle having an aspect ratio of 1.73 and produced in Example 1-2.

[0018] FIG. 6 shows UV-Vis spectrum of the rod-shaped gold nanoparticle having an aspect ratio of 3.59 and produced in Example 1-3.

[0019] FIG. 7 shows a dark field image of the 50 nm-sized circular gold nanoparticle produced in Example 1-1 exposed at 1000 times magnification.

[0020] FIG. 8 shows a dark field image of the rod-shaped gold nanoparticle having an aspect ratio of 1.73 produced in Example 1-2 exposed at 1000 times magnification.

[0021] FIG. 9 shows a dark field image of the rod-shaped gold nanoparticle having an aspect ratio of 3.59 produced in Example 1-3 exposed at 1000 times magnification.

[0022] FIG. 10 shows an HR-TEM image of a mixture in which the 50 nm-sized circular gold nanoparticle, the rod-shaped gold nanoparticle having an aspect ratio of 1.73, and the rod-shaped gold nanoparticle having an aspect ratio of 3.59 are mixed.

[0023] FIG. 11 shows UV-Vis spectrum of the mixture in which the 50 nm-sized circular gold nanoparticle, the rod-shaped gold nanoparticle having an aspect ratio of 1.73, and the rod-shaped gold nanoparticle having an aspect ratio of 3.59 are mixed.

[0024] FIG. 12 shows a dark field image of a mixture in which the 50 nm-sized circular gold nanoparticle, the rod-shaped gold nanoparticle having an aspect ratio of 1.73, and the rod-shaped gold nanoparticle having an aspect ratio of 3.59 are mixed.

[0025] FIG. 13 shows localized surface plasmonic resonance spectrum of the mixture in which the 50 nm-sized circular gold nanoparticle, the rod-shaped gold nanoparticle having an aspect ratio of 1.73, and the rod-shaped gold nanoparticle having an aspect ratio of 3.59 are mixed.

[0026] FIG. 14 shows UV-Vis change spectrum shown for each step in binding PEG and an antibody to the circular gold nanoparticle.

[0027] FIG. 15 shows LSPR light scattering shift spectrum shown for each step in binding PEG and an antibody to the circular gold nanoparticle.

[0028] FIG. 16 shows the LSPR λ_{max} shift of shape-code plasmon biosensors for the independent detection of A β 1-40, A β 1-42 and τ protein.

[0029] FIG. 17A shows linear regression of the calibration curve describing the relationship between the LSPR λ_{max} shifts and A β 1-40, A β 1-42 and τ protein concentrations; and FIG. 17B shows detection of A β 1-40, A β 1-42 and τ protein at concentrations ranging from 10 fM to 10⁸ fM using mimic plasma.

[0030] FIG. 18 shows a detection amount of A β 1-42 according to a concentration of a chaotropic solvent.

[0031] FIG. 19 shows a detection amount of τ protein according to the concentration of the chaotropic solvent.

[0032] FIG. 20 shows a detection amount of A β 1-40 according to the concentration of the chaotropic solvent.

[0033] FIG. 21A shows detection of control (A β 1-40, A β 1-42 and pure plasma) and τ protein at concentrations ranging from 101 fM to 108 fM in plasma; and FIG. 21B shows linear regression of the calibration curve describing the relationship between the LSPR λ_{max} shifts and τ protein concentrations.

[0034] FIG. 22 shows LSPR λ_{max} shifts of nanoplasmonic biosensor for detecting τ protein in cognitive normal control and AD patients' blood samples (Patient No. 1-5) combined with 6M Gua-HCl.

BEST MODE

[0035] Unless defined otherwise, all the technical and scientific terms used herein have the same meanings as those generally understood by persons skilled in the art to which the present invention pertains. In general, nomenclature used in the present specification is well known and generally used in the present technical field.

[0036] The present invention relates to a nanoplasmonic biosensor for diagnosing Alzheimer's disease capable of simultaneously detecting Alzheimer's disease onset markers.

[0037] In the present invention, taking into account the fact that 500 ml of cerebrospinal fluid flows into blood every day, and an onset mechanism of Alzheimer's disease occurring in the brain is fully reflected in the blood, it has been attempted to develop a nanoplasmonic biosensor capable of simultaneously detecting the Alzheimer's disease onset markers in a blood sample.

[0038] In the present invention, each antibody or aptamer that binds to Alzheimer's disease onset marker, A β 1-40 (beta-amyloid 40) peptide, A β 1-42(beta-amyloid 42) peptide, or τ (tau) protein was immobilized to a circular gold nanoparticle, or rod-shaped gold nanoparticles each having an aspect ratio of 1.73 and an aspect ratio of 3.59, and the distinguished optical and visual characteristics of the gold nanoparticles were used to confirm the Alzheimer's disease onset markers. The gold nanoparticles having different shapes and sizes are able to perform colorimetric analysis through surface resonance plasmonic spectrum showing different maximum wavelengths and dark field image. At this time, the antibody or the aptamer of the onset marker was connected by treating heterofunctional polyethylene glycol (SH-PEG-COOH) with the gold nanoparticles. By using the fact that resonance occurs in a larger wavelength region when the gold nanoparticles bind to the onset marker, whether the corresponding onset marker is present was confirmed through a change in spectrum of the nanoparticle that binds to the antibody or the aptamer of the specific onset marker. Meanwhile, it was confirmed that it was possible to quantify the onset marker by standardizing maximum wavelength mobility that occurred when an artificially synthesized marker was applied to a sensor, and thus it was found that the nanoplasmonic biosensor of the present invention was able to detect the Alzheimer's disease onset marker with very high sensitivity and accuracy.

[0039] Accordingly, in an aspect, the present invention provides a method for diagnosing Alzheimer's disease comprising (A) contacting a sample separated from a specimen with a plasmonic sensor based on a gold nanoparticle to which an antibody or an aptamer specific to a target protein of which expression is specifically increased or decreased in Alzheimer's patient is immobilized, thereby inducing a binding between the target protein and the antibody or the aptamer; (B) measuring light scattering spectrum according to the binding; and (C) determining whether or not Alzheimer's disease occurs through analysis of maximum wavelength mobility ($\Delta\lambda_{max}$) obtained from the spectrum.

[0040] In the present invention, the sample may be utilized as long as it is a body fluid discharged from a human body, and it is particularly preferable that the sample is blood in view of the fact that the cerebrospinal fluid flows into the blood.

[0041] In the present invention, the target protein may be one or more selected from the group consisting of A β 1-40(beta-amyloid 40) peptide, A β 1-42(beta-amyloid 42) peptide, and τ (tau) protein, but is not limited thereto.

[0042] In the present invention, non-limiting examples of the antibody or the aptamer specific to A β 1-40(beta-amyloid 40) peptide include anti-beta amyloid 1-40 antibody (abcam, ab20068), anti-beta amyloid 1-40 antibody (abcam, ab12265), beta amyloid (1-40) polyclonal antibody (Invitrogen, 44-136), beta amyloid (1-40) polyclonal antibody (Invitrogen, 44-348A), A beta 40 antibody (Novus bio, NB30-225SS), anti-amyloid beta 1-40 antibody (QED Bioscience Inc., 57002), anti amyloid beta (1-40) (OriGene Technologies, DM410-05), amyloid beta peptide 1-40 (Ab1-40) antibody (Abxexa Ltd., abx132222), anti-amyloid beta peptide 1-40 antibody (MyBioSource.com, MBS2099585), and amyloid beta (1-40/42) antibody (Biorbyt, orb26764).

[0043] In the present invention, non-limiting examples of the antibody or the aptamer specific to τ (tau) protein include tau monoclonal antibody (HT7) (Invitrogen, MN1000), tau antibody (TAU-5) (Santa Cruz, sc-58860), tau, total (TAU-5) (Alzforum, MAB361), tau antibody (TAU-5) (Novus, nb200-514), and tau monoclonal antibody (TAU-5) (absolute antibody).

[0044] In the present invention, non-limiting examples of the antibody or the aptamer specific to A β 1-42(beta-amyloid 42) peptide include anti-beta amyloid 1-42 antibody (Sigma-Aldrich, AB5078P), anti-beta amyloid 1-42 antibody (Abcam, ab12267), anti-beta amyloid 1-42 antibody (Abcam, ab10148) anti-beta amyloid 1-42 antibody (BioLegend, Previously Covance catalog # SIG-39142), anti-beta amyloid 1-42 antibody (Merck (Millipore), AB5078P), and anti-beta amyloid 1-42 antibody (Arigo, ARG11044).

[0045] In the present invention, the gold nanoparticle may differ in shape and/or size depending on a type of antibody or aptamer that is immobilized. In other words, by producing and using gold nanoparticles having different shapes and/or sizes as the number of antibodies or aptamers that bind to each of a plurality of target proteins, various target proteins may be simultaneously detected and thus accuracy of diagnosis of Alzheimer's disease is improved.

[0046] In the present invention, the binding between the target protein and the antibody or the aptamer may be induced in a reaction sample containing a chaotropic solvent, thereby complementing a decrease in detection due to binding between an onset marker present in blood and other proteins. In this case, since the chaotropic solvent has a property of weakening a non-covalent bond between molecules by interfering with arrangement of water molecules present in a solvent, when added to blood, it serves to increase sensitivity of Alzheimer's disease onset marker.

[0047] In the present invention, the binding between the target protein and the antibody or the aptamer may be induced in a reaction sample containing a chaotropic solvent.

[0048] In addition, in the present invention, before inducing a binding between the target protein and the antibody or the aptamer, the blood may be pretreated with a solution containing a chaotropic solvent.

[0049] In the present invention, the chaotropic solvent may be any one selected from the group consisting of guanidine hydrochloride, guanidine thiocyanate, potassium thiocyanate, and sodium trichloroacetate, but is not limited thereto.

[0050] In the present invention, the chaotropic solvent for detection of A β 1-42 is preferably 5M to 7M guanidine hydrochloride or 2M to 5M guanidine thiocyanate, but is not limited thereto.

[0051] In the present invention, the chaotropic solvent for detection of τ protein is preferably 5M to 8M guanidine hydrochloride, more preferably about 6M, or 3.5M to 5.5M guanidine thiocyanate, but is not limited thereto.

[0052] In the present invention, the chaotropic solvent for detection of A β 1-40 is preferably 0.5-3M potassium thiocyanate, 0.5-3M guanidine thiocyanate or 2-8M guanidine hydrochloride, but is not limited thereto.

[0053] In the present invention, the chaotropic solvent for detection of τ protein and A β 1-40 is preferably 5M to 8M guanidine hydrochloride

[0054] In the present invention, the maximum wavelength mobility (i.e. LSPR λ_{max} shift) may be represented by a concentration of an onset factor that binds to a surface of the plasmonic sensor.

[0055] Meanwhile, the present invention also provides a biosensor for detecting Alzheimer's disease in which an antibody or an aptamer of at least any one target protein selected from the group consisting of A β 1-40 peptide, A β 1-42 peptide, and τ protein is immobilized to a gold nanoparticle.

[0056] In the present invention, the gold nanoparticle may differ in shape and/or size depending on a type of the antibody or the aptamer immobilized thereto.

[0057] In the present invention, an average particle size of the gold nanoparticle is preferably 10 to 150 nm, and more preferably 40 to 130 nm. Meanwhile, when the gold nanoparticle has a circular shape, a diameter is preferably 40 to 60 nm, and more preferably about 50 nm, and when the gold nanoparticle has a rod shape, an aspect ratio is preferably 1 to 5, and more preferably 1.6 to 3.7.

[0058] Hereinafter, the present invention will be described in detail with reference to the following Examples. However, the following examples are only for exemplifying the present invention, and it will be obvious to those skilled in the art that the scope of the present invention is not construed to be limited to these examples.

Example 1 Production of Gold Nanoparticle

[0059] In order to produce a nanoplasmonic biosensor based on the surface plasmon resonance phenomenon of the present invention, a 50 nm-sized circular gold nanoparticle, a rod-shaped gold nanoparticle having an aspect ratio of 1.73, and a rod-shaped gold nanoparticle having an aspect ratio of 3.59 were synthesized by a method known in the art (i.e. wet synthesis), and materials used in the synthesis were purchased from Sigma Aldrich (USA).

[0060] 1-1. Production of 50 nm-Sized Circular Gold Nanoparticle

[0061] 10 ml of 0.1M HAuCl₄ and 9.9 ml of sterilized water were mixed in a 20 ml vial and heated at 200° C. while stirring at 1000 to 1500 rpm until boiling. 1 ml of 0.04M sodium citrate was added to the boiled gold aqueous solution, and when the yellow aqueous solution was changed to wine color, the solution was maintained for 5 minutes and then stirred at 1150 rpm at room temperature. After the reaction was completed, the solution was filtered by a 0.2 μ l filter to remove an aggregated product, and a size and a shape were measured by using a high resolution transmission electron microscopy (HR-TEM, JEOL JEM-3011) and a UV/VIS spectrophotometer (UV/VIS 3600, Shimadzu).

[0062] 1-2. Production of Rod-Shaped Gold Nanoparticle Having Aspect Ratio of 1.73

[0063] For a gold nanoparticle seed solution, 5 ml of 0.5 mM HAuCl₄ and 5 ml of 0.2 M CTAB were mixed, and 1 ml of 0.006 M NaBH₄ was added. The Au(III)-CTAB aqueous solution was stirred at 1200 rpm. The seed solution was used after a color of the solution was changed from

yellow to yellowish brown, and the seed solution was aged at room temperature for 30 minutes before use.

[0064] For a growth solution, 1.4 g of CTAB and 0.2468 g of NaOL were dissolved in sterilized water at 50° C., then a temperature of the solution was lowered to 30° C., and 2.4 ml of 4 mM AgNO₃ was added, and the solution was left for 15 minutes without stirring. Then, when 50 ml of 1 mM HAuCl₄ was added and the solution was stirred at 700 rpm for 90 minutes, the color of the aqueous solution disappeared (colorless). 0.3 ml of 37 wt. % (12.1 M) HCl was added and stirred at 400 rpm for 15 minutes to adjust pH. 0.25 ml of 0.064 M ascorbic acid was added and vigorously stirred for 30 seconds, and 0.04 ml of the seed solution was added and vigorously stirred for 30 seconds. Then, the mixture was allowed to grow at 30° C. for 12 hours without stirring. At this time, the color changed to purple. Then, the product was separated by centrifugation at 7000 rpm for 30 minutes, and the supernatant was removed. A size and a shape were measured by using a high resolution transmission electron microscopy (HR-TEM, JEOL JEM-3011) and a UV/VIS spectrophotometer (UV/VIS 3600, Shimadzu).

[0065] 1-3. Production of Rod-Shaped Gold Nanoparticle Having Aspect Ratio of 3.59

[0066] For a gold nanoparticle seed solution, 5 ml of 0.5 mM HAuCl₄ and 5 ml of 0.2 M CTAB were mixed, and 1 ml of 0.006 M NaBH₄ was added. The Au(III)-CTAB aqueous solution was stirred at 1200 rpm. The seed solution was used after a color of the solution was changed from yellow to yellowish brown, and the seed solution was aged at room temperature for 30 minutes before use.

[0067] For a growth solution, 1.8 g of CTAB and 0.2468 g of NaOL were dissolved in sterilized water at 50° C., then a temperature of the solution was lowered to 30° C., and 4.8 ml of 4 mM AgNO₃ was added, and the solution was left for 15 minutes without stirring. Then, when 50 ml of 1 mM HAuCl₄ was added and the solution was stirred at 700 rpm for 90 minutes, the color of the aqueous solution disappeared (colorless). 0.42 ml of 37 wt. % (12.1 M) HCl was added and stirred at 400 rpm for 15 minutes to adjust pH. 0.25 ml of 0.064 M ascorbic acid was added and vigorously stirred for 30 seconds, and 0.04 ml of the seed solution was added and vigorously stirred for 30 seconds. Then, the mixture was allowed to grow at 30° C. for 12 hours without stirring. At this time, the color changed to purple. Then, the product was separated by centrifugation at 7000 rpm for 30 minutes, and the supernatant was removed. A size and a shape were measured by using a high resolution transmission electron microscopy (HR-TEM, JEOL JEM-3011) and a UV/VIS spectrophotometer (UV/VIS 3600, Shimadzu).

[0068] As a result, it was confirmed that the about 50 nm-sized circular gold nanoparticle (FIG. 1), the rod-shaped gold nanoparticle having an aspect ratio of 1.73 (FIG. 2), and the rod-shaped gold nanoparticle having an aspect ratio of 3.59 (FIG. 3) were produced, respectively, and it could be confirmed that different optical and visual characteristics were induced in the circular gold nanoparticle and the rod-shaped gold nanoparticles (FIGS. 4 to 9). Meanwhile, by mixing and observing the circular and rod-shaped gold nanoparticles (FIG. 10), it could be confirmed that surface resonance plasmonic spectrum showing different maximum wavelengths (FIG. 11) and colorimetry through a dark field image (FIG. 12) were observed even in a state in which each of these gold nanoparticles were mixed.

Example 2: Manufacture of Substrate

[0069] A glass substrate which is a support of a nanoplasmonic sensor was surface treated with a silane compound including an amine or alkyl end group. The silane compound was (3-aminopropyl)triethoxysilane, and an amine group was attached to the substrate by immersing the glass substrate in 5% (3-aminopropyl)triethoxysilane solution for 15 minutes.

Example 3: Manufacture of Nanoplasmonic Biosensor Substrate in which Antibody Binds to Circular Gold Nanoparticle

[0070] A circular gold nanoparticle was treated with heterofunctional polyethylene glycol (SH-PEG-COOH), and an antibody with respect to Alzheimer's disease onset marker of A β 1-40 was bound thereto. Here, the used heterofunctional polyethylene glycol (SH-PEG-COOH) had a molecular weight of 2000 and was purchased from Laysan Bio. Ltd. The heterofunctional polyethylene glycol (SH-PEG-COOH) acted as a stabilizer, and provided a functional group that allowed the gold nanoparticle to adhere well to a glass substrate, and further, that was bindable to the antibody. 2 mg of SH-PEG-COOH having a molecular weight of 2000 was dissolved in 1 ml of sterilized water to prepare a solution of 1 mM. Thereafter, 20 μ l of the above prepared solution was added to 1 ml of the 50 nm-sized circular gold nanoparticle aqueous solution synthesized in Example 1-1, stirred for 24 hours, and centrifuged at 7000 rpm for 15 minutes to separate the surface-treated gold nanoparticle. The separated pellet was resuspended in sterilized water to an optical density of 2, and 1 μ l of 0.7 M 1-ethyl-3-(3-dimethylaminopropyl)carbodiimide/N-hydroxysuccinimide (EDC/NHS) was added based on 100 μ l of the gold aqueous solution and mixed well, followed by incubation for 15 minutes. In the meantime, 50 μ l of A β 1-40 antibody (anti-beta amyloid 1-40 antibody (abcam, ab20068); or beta amyloid (1-40) polyclonal antibody (Invitrogen, 44-136)) to be attached to a surface of the gold nanoparticle was diluted with PBS to a concentration of 50 μ g/ml. After 15 minutes, the antibody diluent was added to the PEG-treated gold aqueous solution, and pipetted, and reacted without stirring for 4 hours. After 4 hours, the reaction mixture was centrifuged at 5000 rpm for 10 minutes and redispersed in 100 μ l of sterilized water.

[0071] The antibody-bound circular gold nanoparticle aqueous solution was diluted to an optical density of 0.05, and then 10 μ l of the gold nanoparticle aqueous solution was dropped on the glass substrate. Thereafter, the gold nanoparticle aqueous solution was removed again after about 50 seconds.

[0072] Upon reviewing a change in UV-Vis spectrum wavelength shown for each step in binding the antibody to the circular gold nanoparticle, plasmonic spectrum of the 50 nm-sized circular gold nanoparticle produced in Example 1-1 had a peak at 530.5 nm (FIG. 14, 50 nm bare AuNPs). However, Rayleigh light scattering spectrum of the same single nanoparticle after surface treatment with 1 mM of heterofunctional PEG having a molecular weight of 2000 had a peak at 533 nm (FIG. 14, PEGylated 50 nm AuNPs), and when 50 μ l of antibody at a concentration of 50 μ g/ml was attached to the surface of the gold nanoparticle, and reacted for 4 hours, a peak appeared at 537.2 nm (FIG. 14, 50 μ g/ml antibody binding). In other words, it could be

confirmed that as compared to the circular gold nanoparticle, the UV-Vis maximum wavelength shift of 2.5 nm after the PEG was attached, and the UV-Vis maximum wavelength shift of 4.2 nm after the antibody was attached were observed.

[0073] Meanwhile, in the case of the LSPR light scattering shift spectrum shown for each step in binding the antibody to the circular gold nanoparticle, it could be confirmed that as compared to the plasmonic spectrum of the 50 nm-sized circular gold nanoparticles prepared in Example 1-1 (FIG. 15, 50 nm bare AuNPs), the Rayleigh light scattering spectrum of the same single nanoparticle after surface treatment with 1 mM of heterofunctional PEG having a molecular weight of 2000 (FIG. 15, after SAM) showed the LSPR maximum wavelength shift of 17.3 nm, and the spectrum after 50 μ l of antibody at a concentration of 50 μ g/ml was attached to the surface of the gold nanoparticle (FIG. 15, after ab binding) showed the LSPR λ_{max} shift of 31 nm, respectively.

Example 4: Manufacture of Nanoplasmonic Biosensor in which Antibody Binds to Rod-Shaped Gold Nanoparticle

[0074] A rod-shaped gold nanoparticle was treated with heterofunctional polyethylene glycol (SH-PEG-COOH), and antibodies with respect to two Alzheimer's disease onset markers of A β 1-42 (anti-beta amyloid 1-42 antibody (Abcam, ab10148); or anti-beta amyloid 1-42 antibody (Merck (Millipore), AB5078P)) and τ protein (tau monoclonal antibody (HT7) (Invitrogen, MN1000)) were bound thereto. Here, the used heterofunctional polyethylene glycol (SH-PEG-COOH) had molecular weight of 2000 and 3400, respectively, and purchased from Laysan Bio. Ltd. The heterofunctional polyethylene glycol (SH-PEG-COOH) acted as a stabilizer, and provided a functional group that allowed the gold nanoparticle instead of the CTAB of the surface of the rod-shaped gold nanoparticles having the aspect ratio of 1.73 and 3.59 to adhere well to the glass substrate, and further, that was bindable to the antibody. 53.5 μ l of 300 μ g Au/ml of the rod-shaped gold nanoparticle having the aspect ratio of 3.59 and 50 mg of SH-PEG-COOH having a molecular weight of 3400 were added to 1946.5 μ l of sterilized water. In the case of the rod-shaped gold nanoparticle having the aspect ratio of 1.73, 37.05 μ l of 300 μ g Au/ml of the rod-shaped gold nanoparticle having the aspect ratio of 1.73 and 40 mg of SH-PEG-COOH having a molecular weight of 3400 were added to 1962.95 μ l of sterilized water. The solution was rotation-stirred for 4 days at room temperature to 200 rpm and then centrifuged at 5000 rpm for 4 minutes. The SH-PEG-COOH that did not bind to the gold was removed by the centrifugation, and the solution was resuspended in 1 mL of sterilized water. Then, EDC and NHS were used to connect the gold nanoparticle and the antibody. The rod-shaped gold nanoparticle aqueous solution was diluted to an optical density of 0.1, and then 10 μ l of the gold nanoparticle aqueous solution was dropped on the glass substrate. Thereafter, the gold nanoparticle aqueous solution was removed again after about 5 minutes.

Example 5: Verification of Nanoplasmonic Biosensor Effect

[0075] By using phenomenon that when the gold nanoparticle binds to a biomolecule, resonance occurs in a larger

wavelength region, spectrum changes of the nanoparticle in which the A β 1-40, A β 1-42, and τ protein were bound to the antibody were observed, and whether or not the corresponding Alzheimer's disease onset factor was present was confirmed.

[0076] That is, it was confirmed that the antigen-specific binding was surely generated without cross-talk in the biosensors manufactured in Examples 3 and 4, wherein all the antigens were added at 100 nM, and the PBS was used as a diluting solution.

[0077] In a 50 nm-sized circular gold nanoparticle biosensor manufactured by Example 3, the maximum Rayleigh

gold nanosphere, 26 fM for A β 1-42 with immune-aspect ratio 1.73 of gold nanorod and 23.6 fM for T protein with immune-aspect ratio 3.59 of gold nanorod (FIG. 17B).

Example 6: Enzyme Immunoassay of A β 1-42 According to Chaotropic Solvent

[0079] Ammonium bicarbonate (ABC) was dissolved in water to prepare a 25 mM aqueous solution. Then, guanidine hydrochloride, guanidine thiocyanate, or potassium thiocyanate was dissolved in the 25 mM ammonium bicarbonate (ABC) aqueous solution prepared above to prepare a 20 M stock solution.

TABLE 1

Concentration of a chaotropic solvent for enzyme immunoassay of A β 1-42									
Blood	50 μ L	50 μ L	50 μ L	50 μ L	50 μ L	50 μ L	50 μ L	50 μ L	50 μ L
Diluting Solution	50 μ L	47.5 μ L	45 μ L	40 μ L	35 μ L	30 μ L	25 μ L	20 μ L	10 μ L
guanidine hydrochloride (20M), guanidine thiocyanate (20M) or potassium thiocyanate (20M)	—	2.5 μ L	5 μ L	10 μ L	15 μ L	20 μ L	25 μ L	30 μ L	40 μ L
Final concentration (M)	0	0.5	1	2	3	4	5	6	8

light scattering wavelength shift of about 10 nm was shown for A β 1-40 antibody since it reacted only with 100 nM of A β 1-40 due to the A β 1-40 antibody immobilized to the surface, and the shifts of just 1.4 nm and 1.1 nm were shown for 100 nM of A β 1-42 and τ protein, respectively. Meanwhile, in a rod-shaped gold nanoparticle biosensor having the aspect ratio of 1.73 manufactured by Example 4, since the A β 1-42 was immobilized to the surface of the particle, the maximum scattering wavelength shift of 17 nm was shown for 100 nM A β 1-42, but the maximum scattering wavelength shifts of just about 1.95 nm and 1.93 nm were shown for the A β 1-40 and τ protein at the same concentration, respectively. In addition, in a rod-shaped gold nanoparticle biosensor having the aspect ratio of 3.59 manufactured by Example 4, since the τ protein antibody was immobilized, the maximum scattering wavelength shift of 19 nm was shown for 100 nM T protein, but the maximum scattering wavelength shifts of just about 2.45 nm and 2.5 nm were shown for the two kinds of beta-amyloid and τ protein at the same concentration, respectively (FIG. 16).

[0078] Under biological conditions of patient-mimicked plasma, multiple biomarkers detection was conducted on a platform consisting of three types immunogold with three Alzheimer's disease biomarkers, A β 1-40, A β 1-42 and τ protein. LSPR $\Delta\lambda_{max}$ shifts indicated a strong linearity with the concentration logarithm in the range from 1×10^1 fM to 1×10^8 fM that concentrations are optimized between least twenty times lower and quite higher than levels of biomarkers in AD patient plasma (FIG. 17A). Many coefficients of determination (R^2) were over 0.95 meaning the values of LSPR λ_{max} shift are significantly depended on concentrations of samples in mimicked blood. The limit of detection (LOD) values of the biosensor were calculated by this formula: $LOD = 3 \times \delta / \text{slope}$, where δ is the standard deviation of blank and slope is the slope of calibration curve. Calculated values were 34.9 fM for A β 1-40 with immune 50 nm

[0080] A concentration of the chaotropic solvent was shown above, and analysis was performed according to the instruction of enzyme immunoassay kit (Sensolyte™, Catalog # AS-55552) of A β 1-42. Human blood was used as a sample, and plasma in which an aggregate was removed from the blood was used to perform the experiments.

[0081] To briefly describe the experimental method, a human A β 1-42 standard (Component B) was reconstituted to be 1 ml of peptide standard reconstitution buffer (Component G). In other words, the peptide was hydrated for 10 minutes, reversed upside down and mixed gently. 100 μ L of the reconstituted standard per vial was dispensed and stored at -80° C. before use.

[0082] The strips (Component A) were aligned and labeled according to the number of wells used in the standard and the sample, and then the dilution standard and the sample were each subjected to duplicate dispensing. Sequential dilution of the human A β 1-42 standard was prepared immediately before the experiment, and proceeded as described in Table 2 below.

TABLE 2

Step	Concentration, pg/mL	A β 42 Standard (Component B)	Sample Dilution Buffer (Component C)
1	1,000,000	Prepare as described in 1.1	
2	10,000	10 μ L from step 1	990 μ L
3	250	25 μ L from step 2	975 μ L
4	125	500 μ L from step 3	500 μ L
5	62.5	500 μ L from step 4	500 μ L
6	31.25	500 μ L from step 5	500 μ L
7	15.625	500 μ L from step 6	500 μ L
8	7.8125	500 μ L from step 7	500 μ L
9	3.91	500 μ L from step 8	500 μ L

[0083] A detection antibody (Component H) was diluted 200-fold with a detection antibody dilution buffer (Compo-

nent I). 50 μ l of the antibody solution was dispensed into each well, and 100 μ l of the diluted A β 1-42 standard including the blank was subjected to duplicate dispensing into each well. Meanwhile, 100 μ l of the diluted sample as shown in Table 1 above was added to each well, and 50 μ l of the antibody solution was added to each well. The plate was covered with an adhesive plate cover (Component J) and allowed to react by blocking light at 4° C. overnight. A

Example 7: Enzyme Immunoassay of τ Protein According to Chaotropic Solvent

[0085] Ammonium bicarbonate (ABC) was dissolved in water to prepare a 25 mM aqueous solution. Then, guanidine hydrochloride, guanidine thiocyanate, and potassium thiocyanate were dissolved in the 25 mM ammonium bicarbonate (ABC) aqueous solution prepared above to prepare a 20 M stock solution.

TABLE 3

Concentration of a chaotropic solvent(guanidine hydrochloride) for enzyme immunoassay of τ protein									
Blood	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l
Diluting Solution	50 μ l	47.5 μ l	45 μ l	40 μ l	35 μ l	30 μ l	25 μ l	20 μ l	10 μ l
Guanidine hydrochloride (20M)	—	2.5 μ l	5 μ l	10 μ l	15 μ l	20 μ l	25 μ l	30 μ l	40 μ l
Final concentration (M)	0	0.5	1	2	3	4	5	6	8

TABLE 4

Concentration of a chaotropic solvent(guanidine thiocyanate) for enzyme immunoassay of τ protein									
Blood	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l
Diluting Solution	50 μ l	47.5 μ l	45 μ l	40 μ l	35 μ l	30 μ l	25 μ l	20 μ l	10 μ l
guanidine thiocyanate (20M)	—	2.5 μ l	5 μ l	10 μ l	15 μ l	20 μ l	25 μ l	30 μ l	40 μ l
Final concentration (M)	0	0.5	1	2	3	4	5	6	8

TABLE 5

Concentration of a chaotropic solvent(potassium thiocyanate) for enzyme immunoassay of τ protein									
Blood	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l
Diluting Solution	50 μ l	47.5 μ l	45 μ l	40 μ l	35 μ l	30 μ l	25 μ l	20 μ l	10 μ l
potassium thiocyanate (20M)	—	2.5 μ l	5 μ l	10 μ l	15 μ l	20 μ l	25 μ l	30 μ l	40 μ l
Final concentration (M)	0	0.5	1	2	3	4	5	6	8

10 \times wash buffer (Component D) was diluted with distilled water to prepare a 1 \times wash buffer, the solution of the plate reacted overnight was removed, and the plate was washed 6 to 7 times in each well using 350 μ l of 1 \times wash buffer. Between each wash process before the wash solution was removed, time was taken to allow the wash buffer to fully act for 20 seconds. The plate was cleaned using a paper towel for accurate optical reading. 100 μ l of TMB color substrate solution (Component E) was added to each well, and the plate was lightly tapped and reacted at room temperature for about 5 to 15 minutes until a blue color gradient appeared along the well. 50 μ l of termination solution (Component F) was added to each well and the plate was tapped lightly to turn blue color to yellow. Absorbance (OD) was measured at 450 nm using a microplate absorbance reader within 20 minutes after the termination solution was added.

[0084] As a result, it could be confirmed that a detection amount of A β 1-42 was higher in 6M guanidine hydrochloride or 3M to 4M guanidine thiocyanate (FIG. 18).

[0086] A concentration of the chaotropic solvent was shown above, and analysis was performed according to the instruction of enzyme immunoassay kit (Invitrogen, Catalog nos. KHB0041, KHB0042) of τ protein. Human blood was used as a sample, and plasma in which the aggregate was removed from the blood was used to perform the experiments.

[0087] To briefly describe the experimental method, except for a chromogenic blank, 100 μ l of a standard dilution buffer was added to a zero well. 100 μ l of standard was added to an appropriate well for a standard curve, and 50 μ l of sample and 50 μ l of standard dilution buffer were added to a well for sample analysis. The plate was covered with a cover and allowed to react at room temperature for 2 hours, the solution was thoroughly removed by aspiration, and the plate was washed 4 times with 1 \times wash buffer. Then, 100 μ l of human FGF-b Biotin conjugate solution was added to each well except the chromogenic blank, and mixed by tapping the side of the plate lightly. The plate was covered with a cover and allowed to react at room temperature for 1 hour, the solution was thoroughly removed by aspiration,

TABLE 8

Concentration of a chaotropic solvent(potassium thiocyanate) for enzyme immunoassay of A β 1-40									
Blood	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l	50 μ l
Diluting Solution	50 μ l	47.5 μ l	45 μ l	40 μ l	35 μ l	30 μ l	25 μ l	20 μ l	10 μ l
potassium thiocyanate (20M)	—	2.5 μ l	5 μ l	10 μ l	15 μ l	20 μ l	25 μ l	30 μ l	40 μ l
Final concentration (M)	0	0.5	1	2	3	4	5	6	8

[0091] A concentration of the chaotropic solvent was shown above, and analysis was performed according to the instruction of enzyme immunoassay kit (Cusabio, Catalog no. CSB-E08299h) of A β 1-40. Human blood was used as a sample, and plasma in which the aggregate was removed from the blood was used to perform the experiments.

[0092] A detection amount of A β 1-40 according to the concentration of chaotropic solvent was confirmed, and as a result, it could be confirmed that the detection amount of A β 1-40 increased in all cases where the chaotropic solvent was used, and among them, the detection amount of A β 1-40 increased in the case where 2 M to 3 M of potassium

tein was stained by immersion with 50 ml of 10 times diluted brilliant blue G solution. Here, the protein was stained for 13 hours while shaking at 50 rpm on an orbital shaker, and rinsed with sterilized water until bands were visible after staining.

[0094] Meanwhile, ammonium bicarbonate (ABC) was dissolved in water to prepare a 25 mM aqueous solution. Then, guanidine hydrochloride, guanidine thiocyanate, and potassium thiocyanate were dissolved in the 25 mM ammonium bicarbonate (ABC) aqueous solution prepared above to prepare a 20 M stock solution. The stock solution was used to prepare a sample, followed by electrophoresis.

TABLE 9

Blood	10 μ l	5 μ l	5 μ l	5 μ l	5 μ l	5 μ l	5 μ l	5 μ l	5 μ l
Diluting Solution (Tris-glycine buffer)	—	47.5 μ l	4.5 μ l	4 μ l	3.5 μ l	3 μ l	2.5 μ l	2 μ l	1 μ l
chaotropic solvent (20M)	—	0.25 μ l	0.5 μ l	1 μ l	1.5 μ l	2 μ l	2.5 μ l	3 μ l	4 μ l
final concentration	0	0.5	1	2	3	4	5	6	8

thiocyanate was used and in the case where 6 M of guanidine hydrochloride was used (FIG. 20).

Example 9: Analysis of Alzheimer's Disease Onset Marker According to Chaotropic Solvent by Polyacrylamide Gel Electrophoresis

[0093] For CAST GEL, an acrylamide content was determined according to the molecular weight of Alzheimer's disease onset markers. 15% Tris-glycine polyacrylamide gel was prepared with reference to the molecular weight of about 4 kDa in A β 1-40 and A β 1-42, and the molecular weight of about 36.8 to 45.9 kDa according to the isoform in T protein. 15% Tris-glycine polyacrylamide gel was prepared by mixing 2.3 ml of sterilized water, 5.0 ml of 30% acrylamide mix, 2.5 ml of 1.5 M Tris buffer (pH 8.8), 0.1 ml of 10% ammonium persulfate, and 0.004 ml of TEMED. A stacking gel was prepared by mixing 2.7 ml of sterilized water, 0.67 ml of 30% acrylamide mix, 0.5 ml of 1.0 M Tris buffer (pH 6.8), 0.04 ml of 10% ammonium persulfate, and 0.004 ml of TEMED. The prepared gel solutions were put sequentially in a gel caster and casted. While the gel was solidified, a 10 \times Tris-glycine buffer was diluted, and the sample and a protein weight standard marker were prepared. Here, if dilution of the sample was necessary, 1 \times Tris-glycine buffer was used. When the gel preparation was completed, the standard marker was put on the first line, the samples were set on the other lines and loaded at 20V for about 10 hours. Then, a stacking gel portion was cut off and removed from the polyacrylamide gel, and the loaded pro-

Example 10. Confirmation of Nanoplasmonic Biosensor in AD Patient Sample

[0095] We confirmed the medical usefulness of this nanoplasmonic biosensor that was assisted by a chaotrope for the diagnosis of AD from the blood samples of patients (FIG. 22). We also proved that this highly sensitive platform distinguishes between normal control and AD patients. The plasma samples were obtained from pooled normal human plasma and AD human plasma (Innovative Research Inc., Novi, Mich.). The patients had been clinically diagnosed as AD, and this status continues (mean age: 72.6 \pm 6.3; 3 women, 2 men). We measured the Rayleigh scattering shifts of τ protein-specific immunogold before/after the injection of cognitive normal control plasma and the patients' samples (Patient No. 1-5), with or without 6 M Gua-HCl. The concentration of τ protein in blood is high in patients with Alzheimer's disease.10,18,19 In cases 1, 4 and 5, the LSPR λ_{max} shift values were lower than that of the control when the chaotrope was not used (Black bars in FIG. 22). The assay without the chaotrope did not discriminate between AD and control patients. In contrast, the combination of the plasmon biosensor and the chaotrope resulted in the assays of patients having a higher LSPR λ_{max} shift than those of controls with the chaotrope (Grey bars in FIG. 22). The chaotrope partly disassembled aggregated τ proteins in blood 41 and uncovered the τ protein epitope from blood proteins. The biosensor could therefore react with all of the τ protein in blood, and its accuracy and sensitivity for the diagnosis of AD was enhanced with 6 M Gua-HCl. Plasma

τ protein levels were significantly higher in subjects with AD than controls. The average Rayleigh scattering peak shifts were 8.96 ± 0.93 nm after the injection of AD plasma with 6 M Gua-HCl and 5.9 ± 1.07 nm for controls with the chaotrope (FIG. 22). This finding was supported by studies that showed that τ protein concentrations in plasma samples increased in the order from subjects with normal control and mild cognitive impairment (MCI) to AD and early-stage AD patients.^{15,18,23} Additionally, AD plasma τ protein levels were negatively associated with the most valuable imaging diagnosis factors, including total hippocampus volume and the grey matter density of the superior frontal gyrus.^{47,48} Other regression analyses as well as the identified negative association of cognitive functions and plasma T protein levels have been proven to correlate to delayed recall of logical memory and verbal fluency.¹⁸ On the other hand, the two A β isoforms did not differentiate between AD and control patients even though we demonstrated the high sensitivity of a nanoplasmonic biosensor with chaotropes. Recent studies have also shown that plasma A β and 42 levels are similar in AD and control groups. These findings sustain the idea that only plasma τ protein can provide insights regarding this pathological process in brain. Our proposed system is an optimized clinical assay to accurately diagnose AD patients by the precise detection of τ protein in plasma and reducing the overlapping range between concentrations of the protein in an age-matched control and AD patients' blood that presented a problem in prior studies. This combined use of a nanoplasmonic biosensor and a chaotropic agent provides a precise medical investigational method to determine the core pathophysiology of AD in blood and to distinguish AD patients with high accuracy.

[0096] The method for diagnosing Alzheimer's disease according to the present invention is able to diagnose Alzheimer's disease by using blood that is easily obtainable from the human body, and thus it is possible to perform objective analysis without requiring a complicated surgical procedure for diagnosing Alzheimer's disease. Further, by applying the gold nanoparticles having various sizes and shapes, it is possible to confirm multiple onset markers on a single platform to thereby achieve multiple detection, and by pretreatment of the chaotropic solvent in order to compensate for the decrease in detectability caused when the onset marker present in blood binds to other proteins, it is possible to improve sensitivity of the diagnosis.

[0097] The present invention has been described in detail based on particular features thereof, and it is obvious to those skilled in the art that these specific technologies are merely preferable embodiments and thus the scope of the present invention is not limited to the embodiments. Therefore, the substantial scope of the present invention is defined by the accompanying claims and equivalent thereof.

1. A method for diagnosing Alzheimer's disease in a subject suffering the same comprising the steps of:

- (A) pretreating a blood sample from the subject with a solution comprising a chaotropic solvent comprising 6M guanidine hydrochloride;
- (B) contacting the pretreated blood sample with a plasmonic sensor based on a plurality of gold nanoparticles to which τ protein antibody is immobilized;
- (C) measuring a light scattering spectrum of the blood sample upon contacting with the plasmonic sensor; and
- (D) determining whether the Alzheimer's disease occurs in response to analysis of maximum wavelength mobility ($\Delta\lambda_{max}$) obtained from the light scattering spectrum.

2. A biosensor for detecting Alzheimer's disease comprising:

- τ protein antibody immobilized to a plurality of gold nanoparticles; and
- a solution comprising a chaotropic solvent comprising 6M guanidine hydrochloride.

3. A method for detecting Alzheimer's disease onset markers in a subject suffering Alzheimer's disease comprising the steps of:

- (A) pretreating a blood sample from the subject with a solution comprising a chaotropic solvent;
- (B) contacting the pretreated blood sample with a plasmonic sensor based on a plurality of gold nanoparticles to which one or more antibodies selected from a group consisting of A β 1-40 antibody and τ protein antibody, are immobilized;
- (C) measuring a light scattering spectrum of the blood sample upon contacting with the plasmonic sensor; and
- (D) detecting the Alzheimer's disease onset markers in response to analysis of maximum wavelength mobility ($\Delta\lambda_{max}$) obtained from the light scattering spectrum, wherein the Alzheimer's disease onset markers are selected from a group consisting of A β 1-40 peptide and τ protein,

wherein when the one or more antibodies is the A β 1-antibody, then 0.5-3M potassium thiocyanate, 0.5-3M guanidine thiocyanate or 2-8M guanidine hydrochloride is used as the chaotropic solvent,

wherein when the one or more antibodies is the τ protein antibody, then 5-8M guanidine hydrochloride or 3.5-5.5M guanidine thiocyanate is used as the chaotropic solvent, and

wherein when the one or more antibodies are the A β 1-antibody and the τ protein antibody, then 5-8M guanidine hydrochloride is used as the chaotropic solvent.

4. The method of claim 3, wherein an aspect ratio of the gold nanoparticle to which the A β 1-40 antibody is immobilized, an aspect ratio of the gold nanoparticle to which τ protein antibody is immobilized, an aspect ratio of the gold nanoparticle to which the A β 1-40 antibody and τ protein antibody are immobilized, are different from each other.

* * * * *

专利名称(译)	瑞利散射和金纳米颗粒比色测定的生物传感器用于阿尔茨海默氏病的诊断以及生物传感器的多检测方法		
公开(公告)号	US20200124596A1	公开(公告)日	2020-04-23
申请号	US16/686610	申请日	2019-11-18
发明人	SIM, SANGJUN		
IPC分类号	G01N33/543 G01N33/531 G01N33/68 G01N21/25		
CPC分类号	G01N33/54393 B82Y5/00 G01N2800/2821 G01N33/531 G01N21/25 G01N33/6896 B82Y15/00 G01N2021/258 G01N33/54346		
外部链接	Espacenet USPTO		

摘要(译)

纳米等离子体传感器技术领域本发明涉及一种基于金纳米粒子的纳米等离子体传感器，所述金纳米粒子与抗体或适体结合，该抗体或适体识别存在的阿尔茨海默氏病发作标志物A β 1-40，A β 1-42和 τ 蛋白。在血液中，以及使用瑞利散射现象和传感器的比色测定的阿尔茨海默氏病多检测方法。本发明的优点在于，可以通过使用血液的简单诊断方法对各种发作标记同时进行多次检测，并且通过使用离液溶剂提高诊断的灵敏度。

