



US 20080176253A1

(19) **United States**

(12) **Patent Application Publication**
Christodoulides et al.

(10) **Pub. No.: US 2008/0176253 A1**
(43) **Pub. Date: Jul. 24, 2008**

(54) **DETECTING HUMAN OR ANIMAL IMMUNOGLOBIN-E**

(22) Filed: **May 10, 2007**

Related U.S. Application Data

(75) Inventors: **Nicolaos Christodoulides**, Austin, TX (US); **Pierre N. Floriano**, Austin, TX (US); **Karri Ballard**, Pflugerville, TX (US); **John T. McDevitt**, Austin, TX (US)

(60) Provisional application No. 60/799,609, filed on May 10, 2006.

Publication Classification

Correspondence Address:
FULBRIGHT & JAWORSKI L.L.P.
600 CONGRESS AVE., SUITE 2400
AUSTIN, TX 78701


(51) **Int. Cl.**
G01N 33/53 (2006.01)
C12M 1/00 (2006.01)
(52) **U.S. Cl.** **435/7.21; 435/287.2**


(57) **ABSTRACT**

(73) Assignee: **THE BOARD OF REGENTS OF THE UNIVERSITY OF TEXAS SYSTEM**

Methods, systems, and apparatus for detecting the presence of human or animal immunoglobulin-E are described. A fluid or gas sample may pass through a particle-based detection system of a cartridge. Detection and analysis techniques may be applied to determine the identity and quantity of the captured IgE.

(21) Appl. No.: **11/746,941**

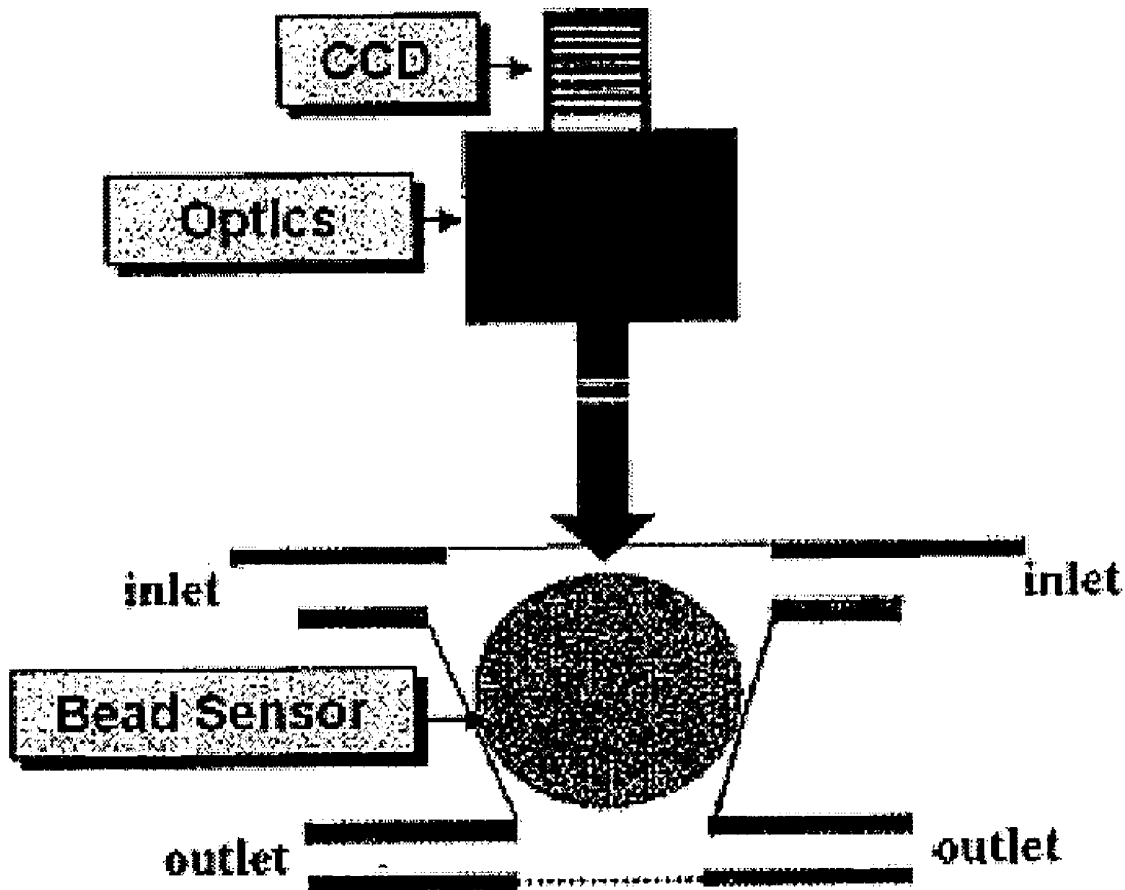

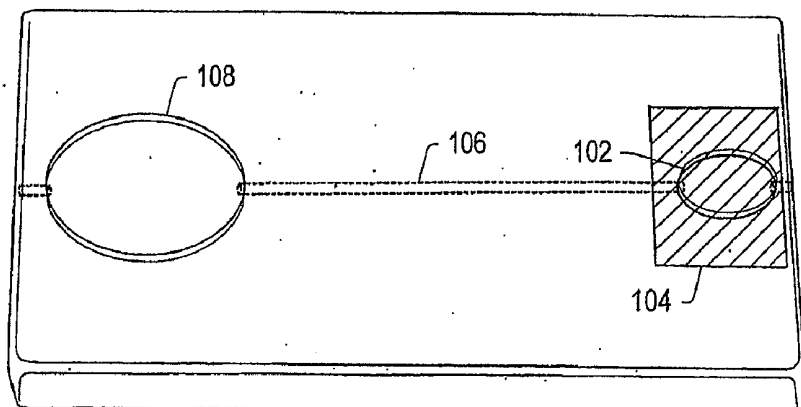

100 ↗

FIG. 1

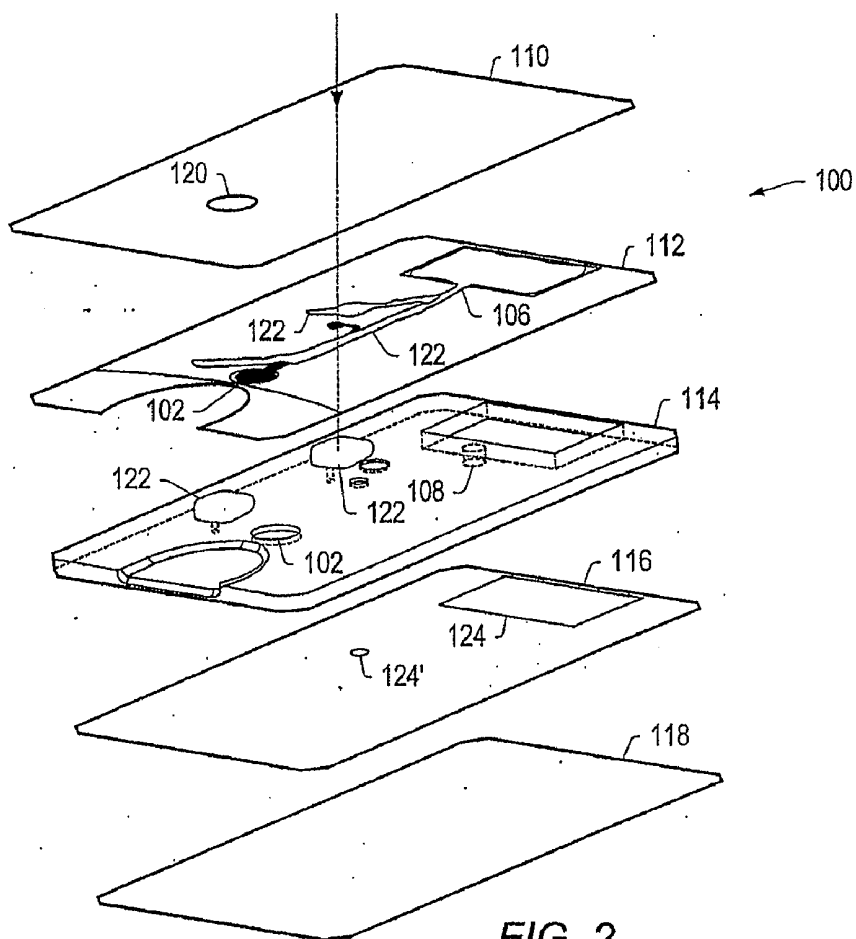


FIG. 2

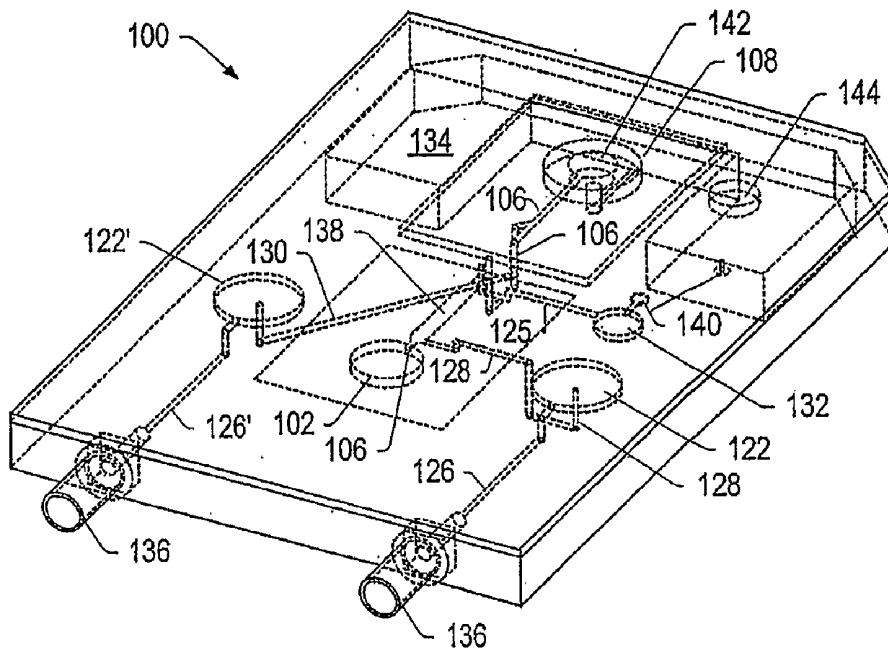


FIG. 3

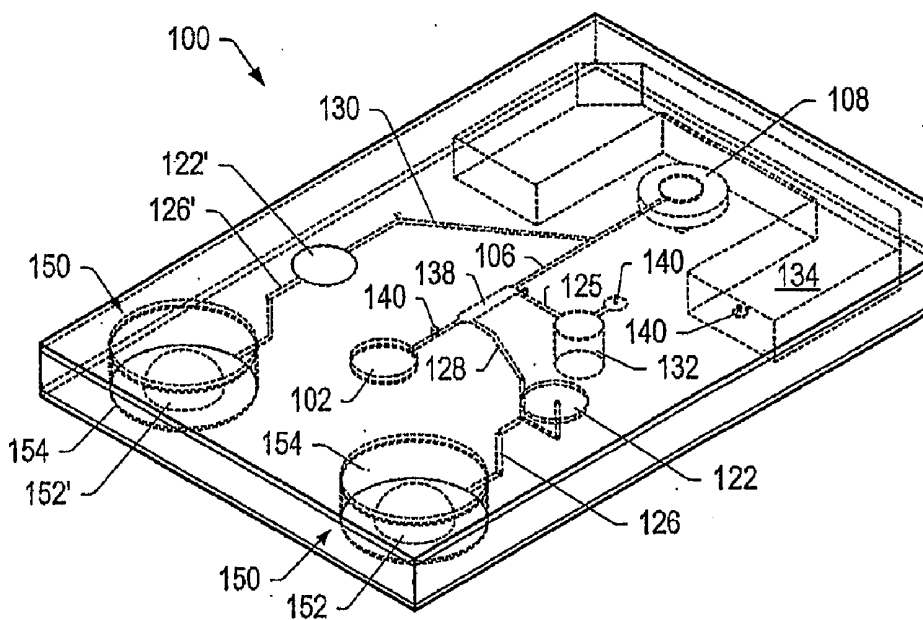


FIG. 4

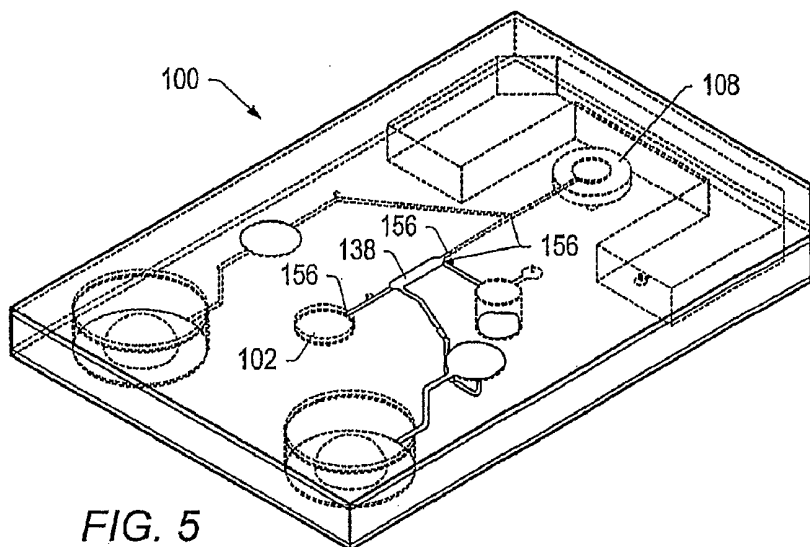


FIG. 5

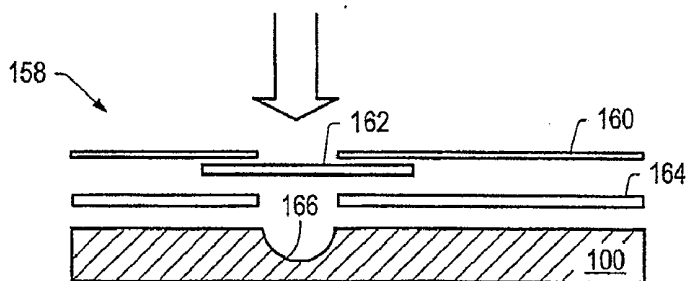


FIG. 6

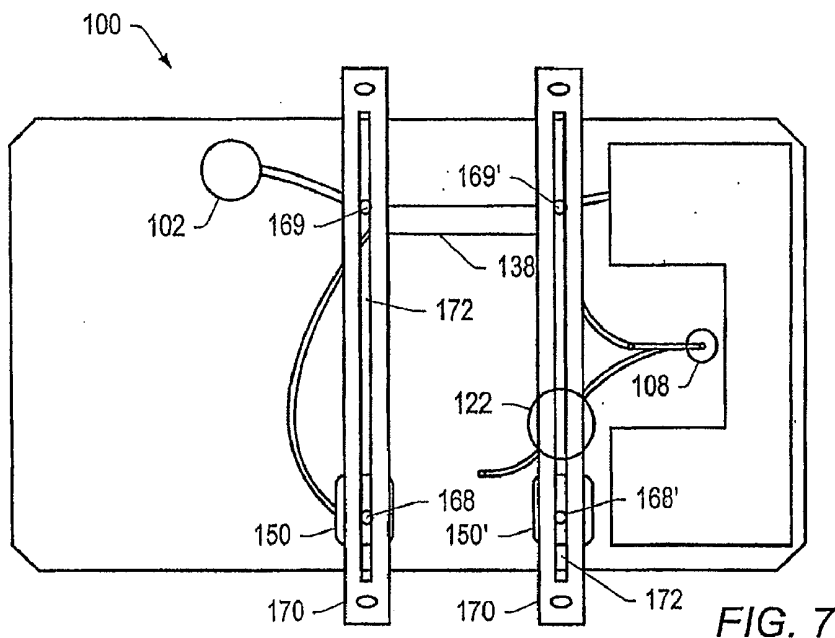


FIG. 7

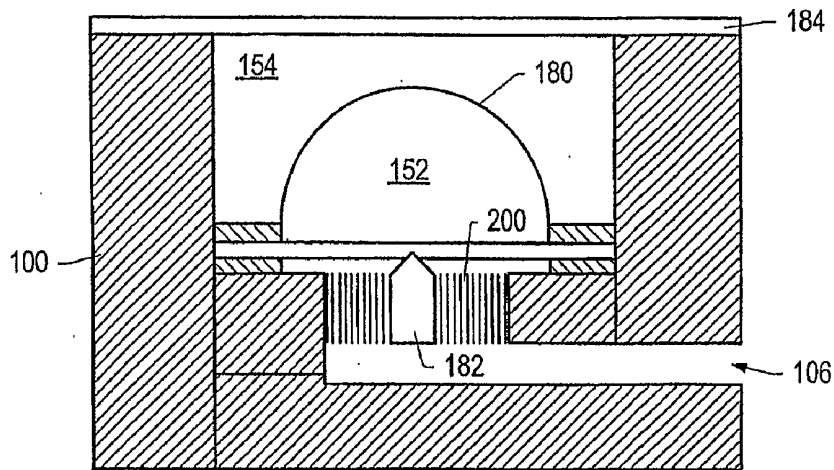
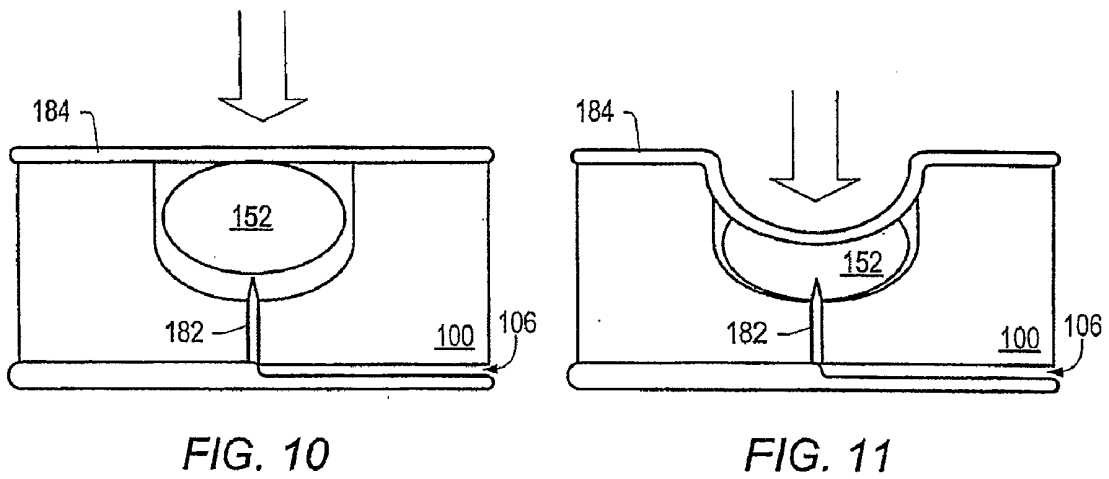
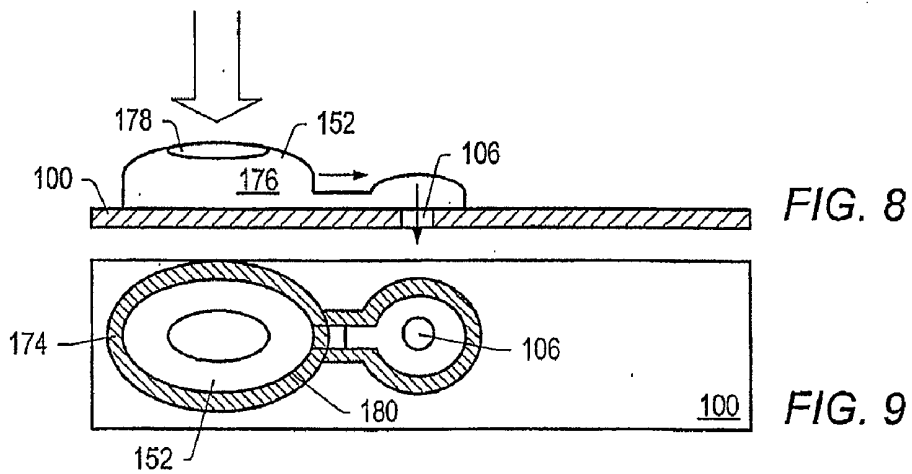


FIG. 12

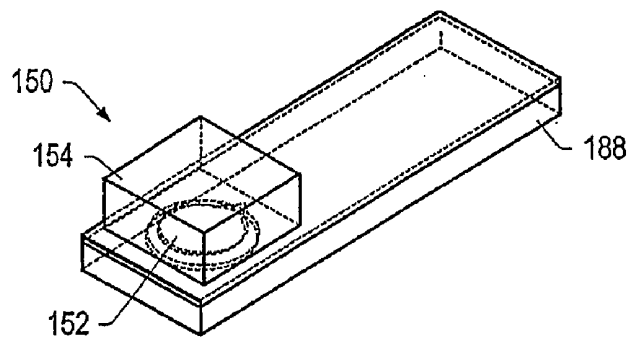


FIG. 13

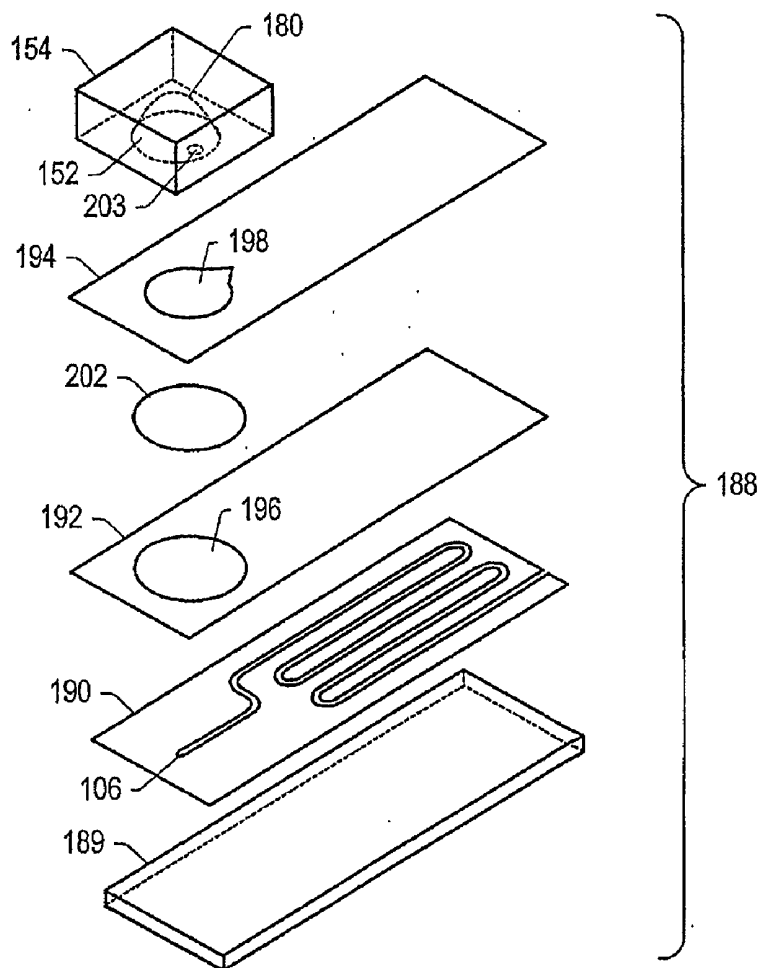


FIG. 14

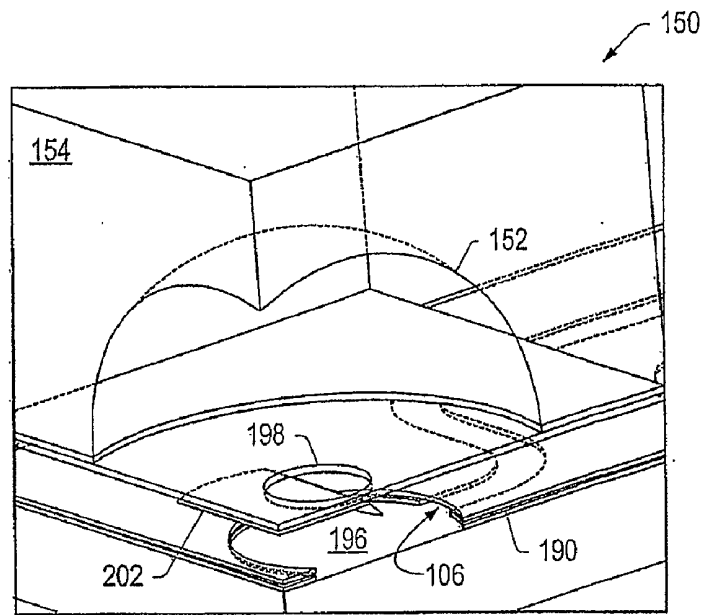


FIG. 15

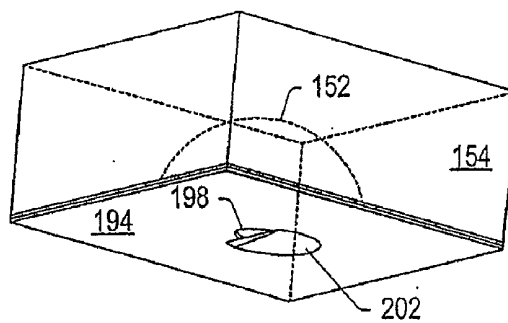


FIG. 16




FIG. 17

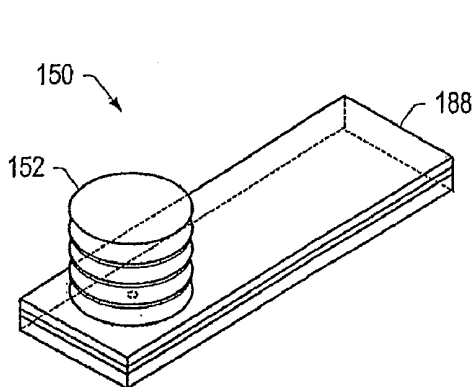


FIG. 18

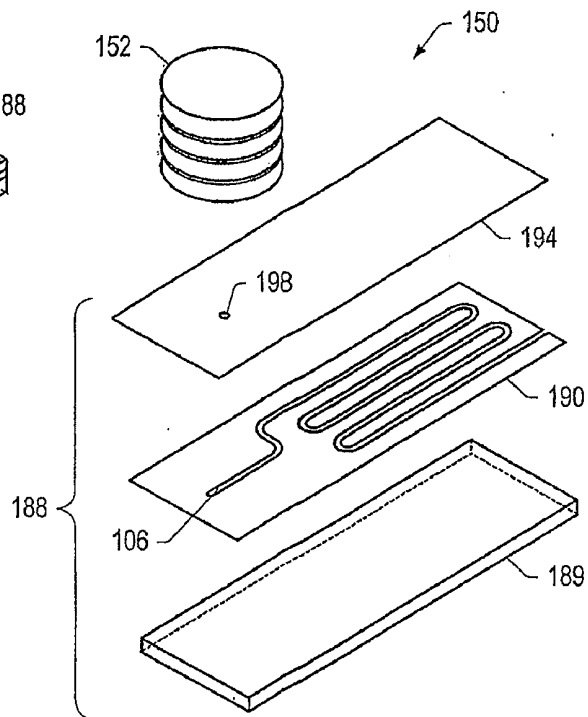


FIG. 19

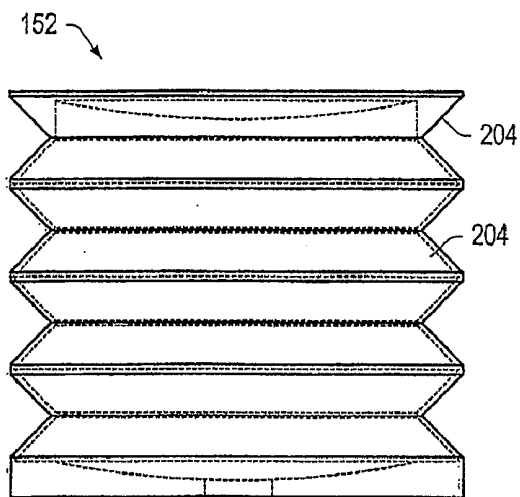


FIG. 20

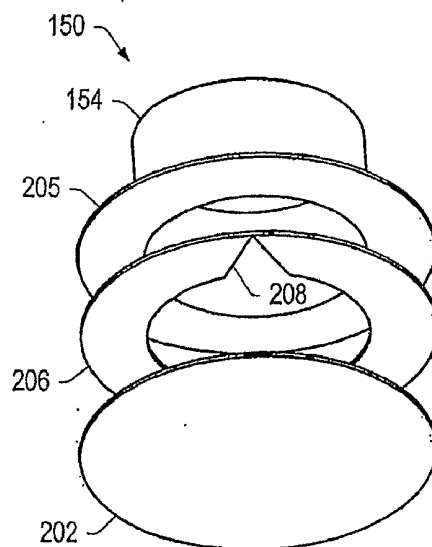


FIG. 21

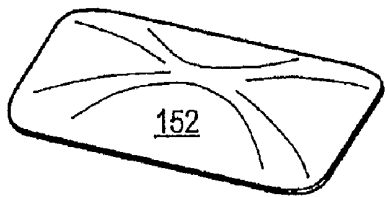


FIG. 22A

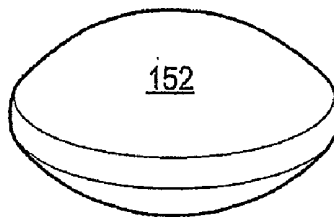


FIG. 22B

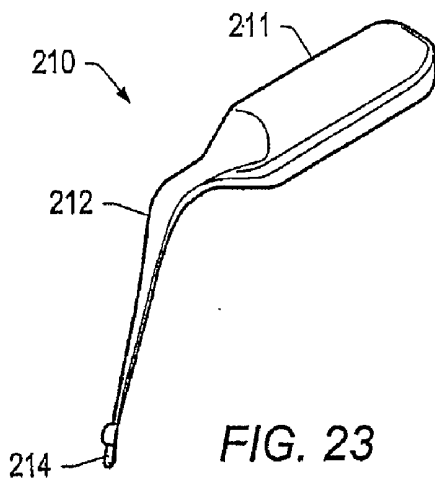


FIG. 23

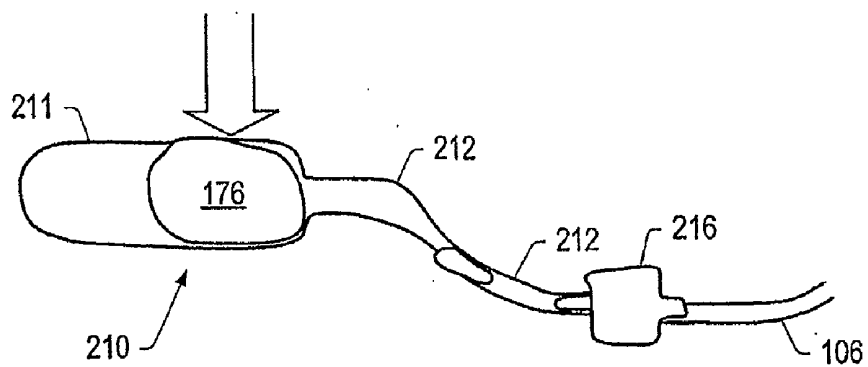


FIG. 24

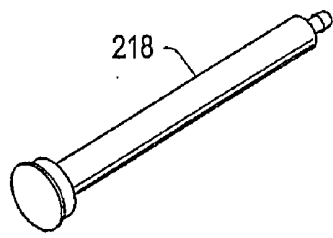


FIG. 25A




FIG. 25B




FIG. 25C




FIG. 25D




FIG. 25E




FIG. 25F




FIG. 25G

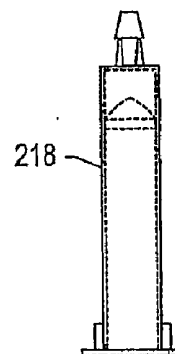


FIG. 25H

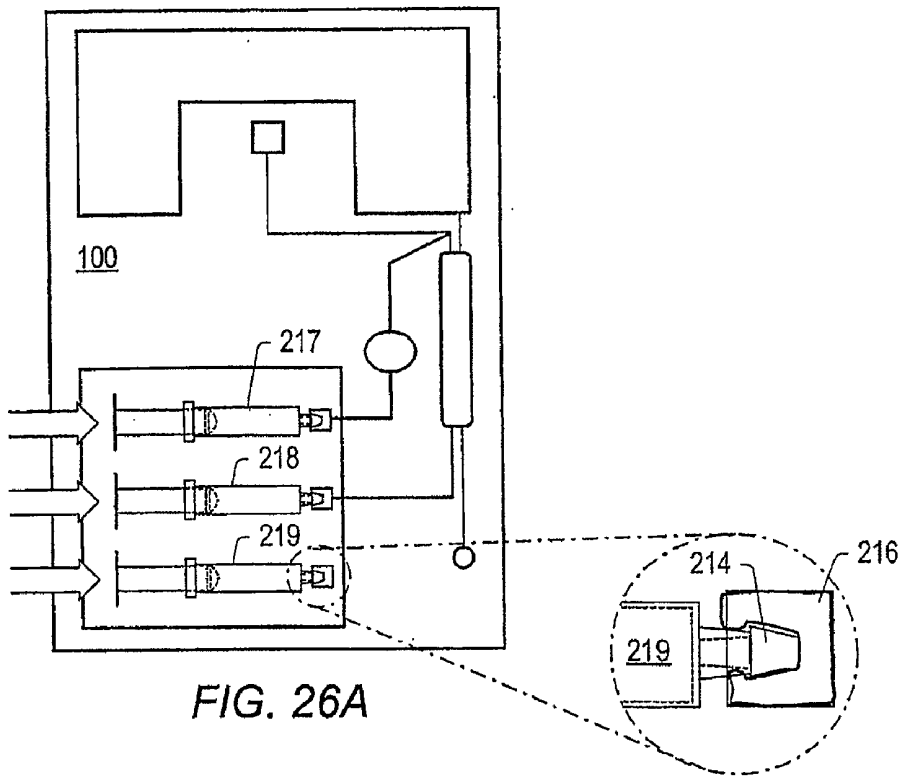


FIG. 26A

FIG. 26B

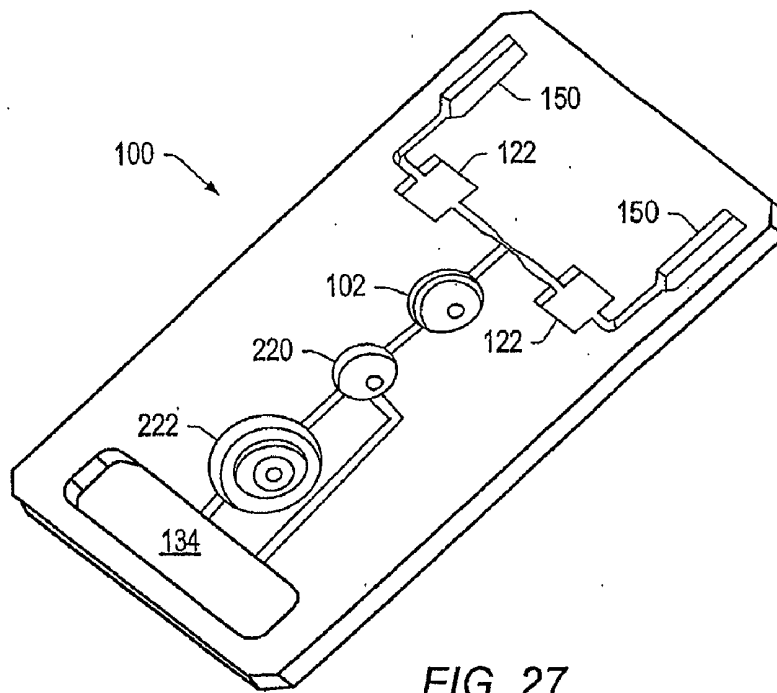


FIG. 27

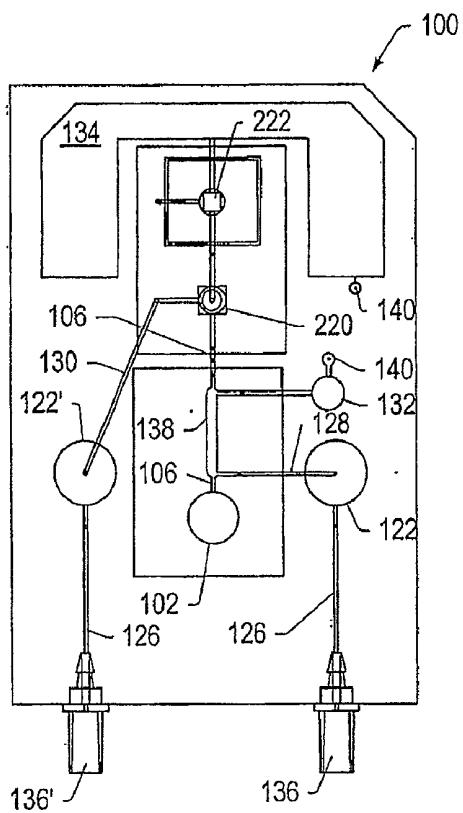


FIG. 28

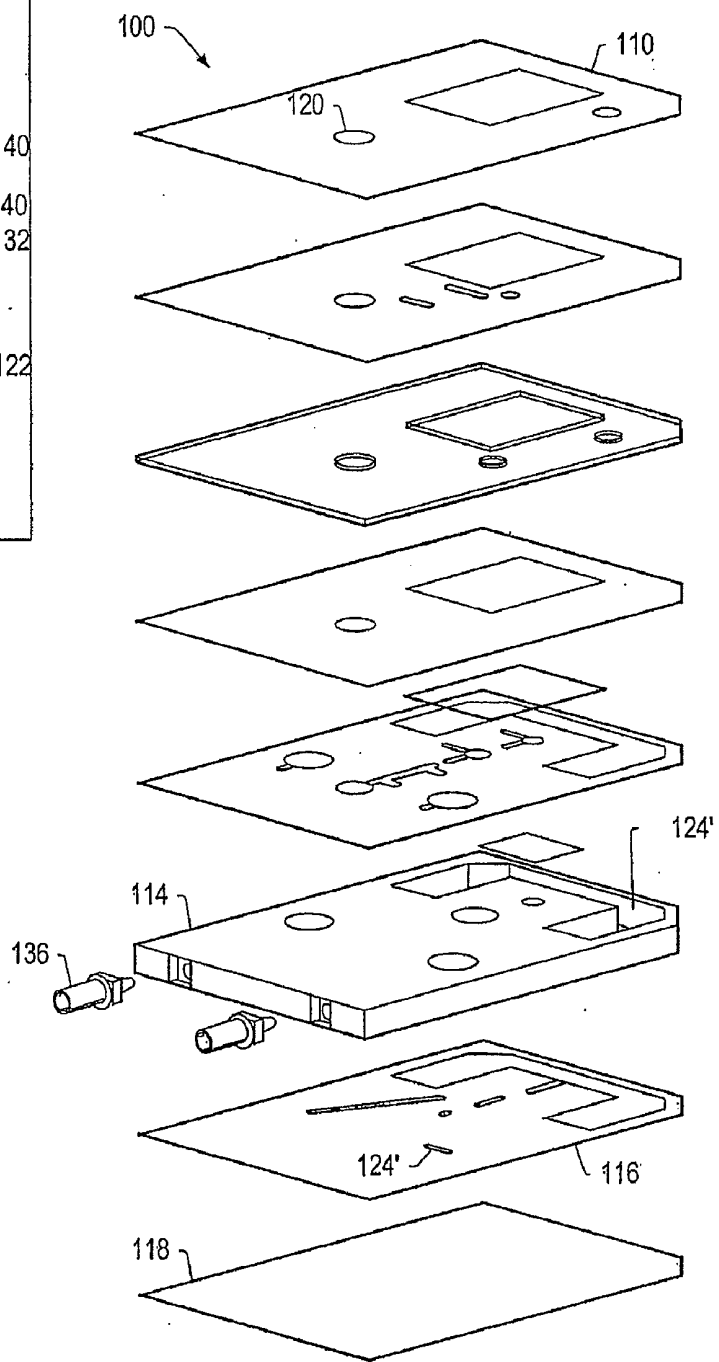


FIG. 29

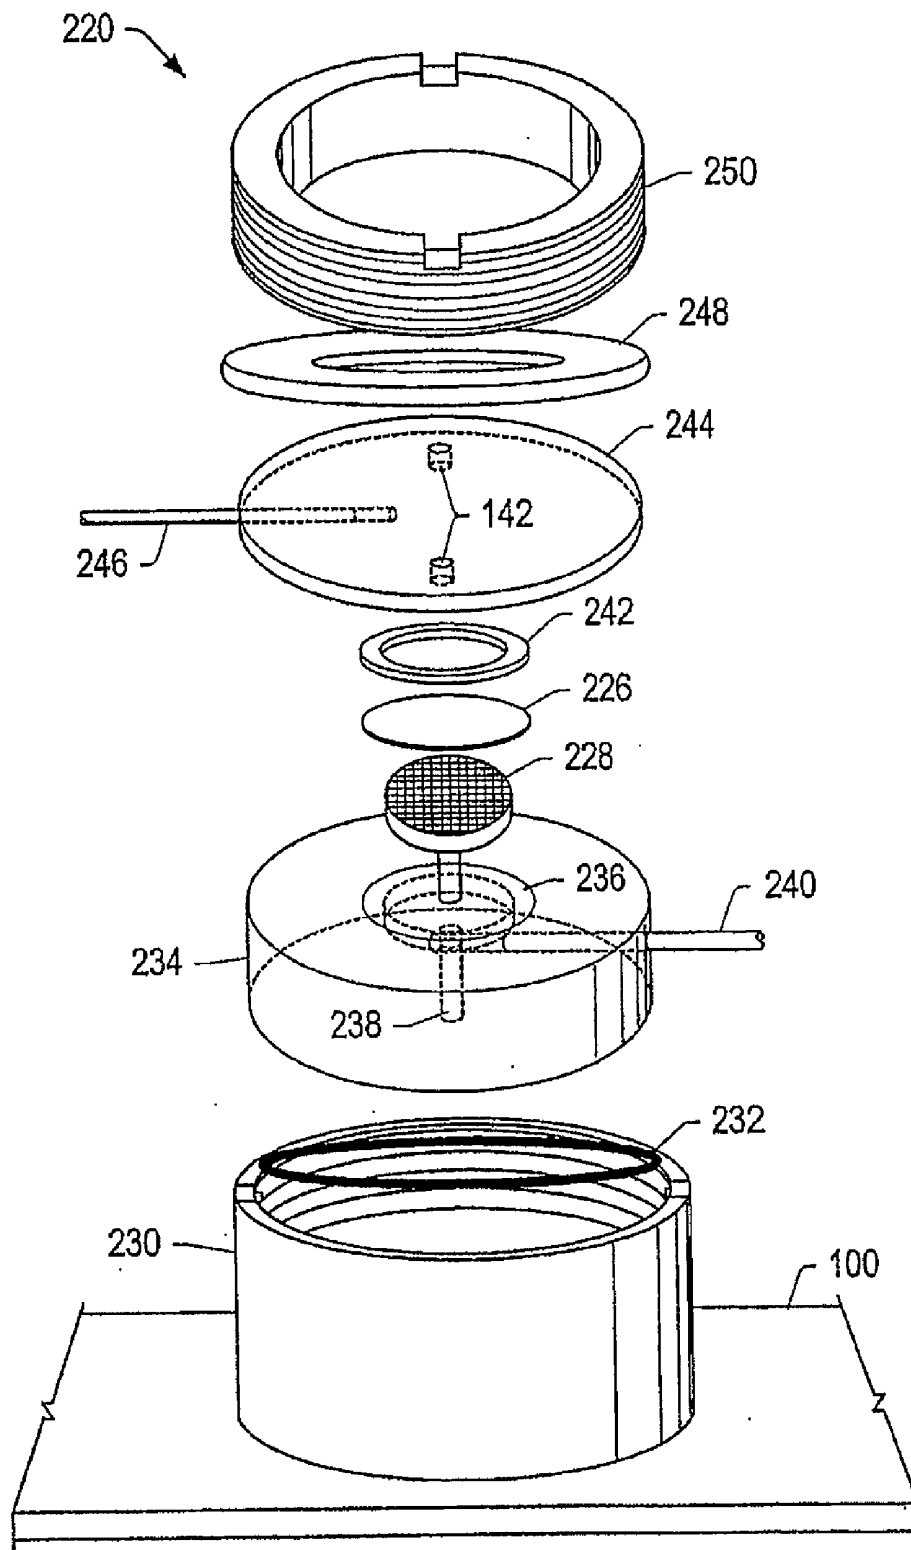


FIG. 30

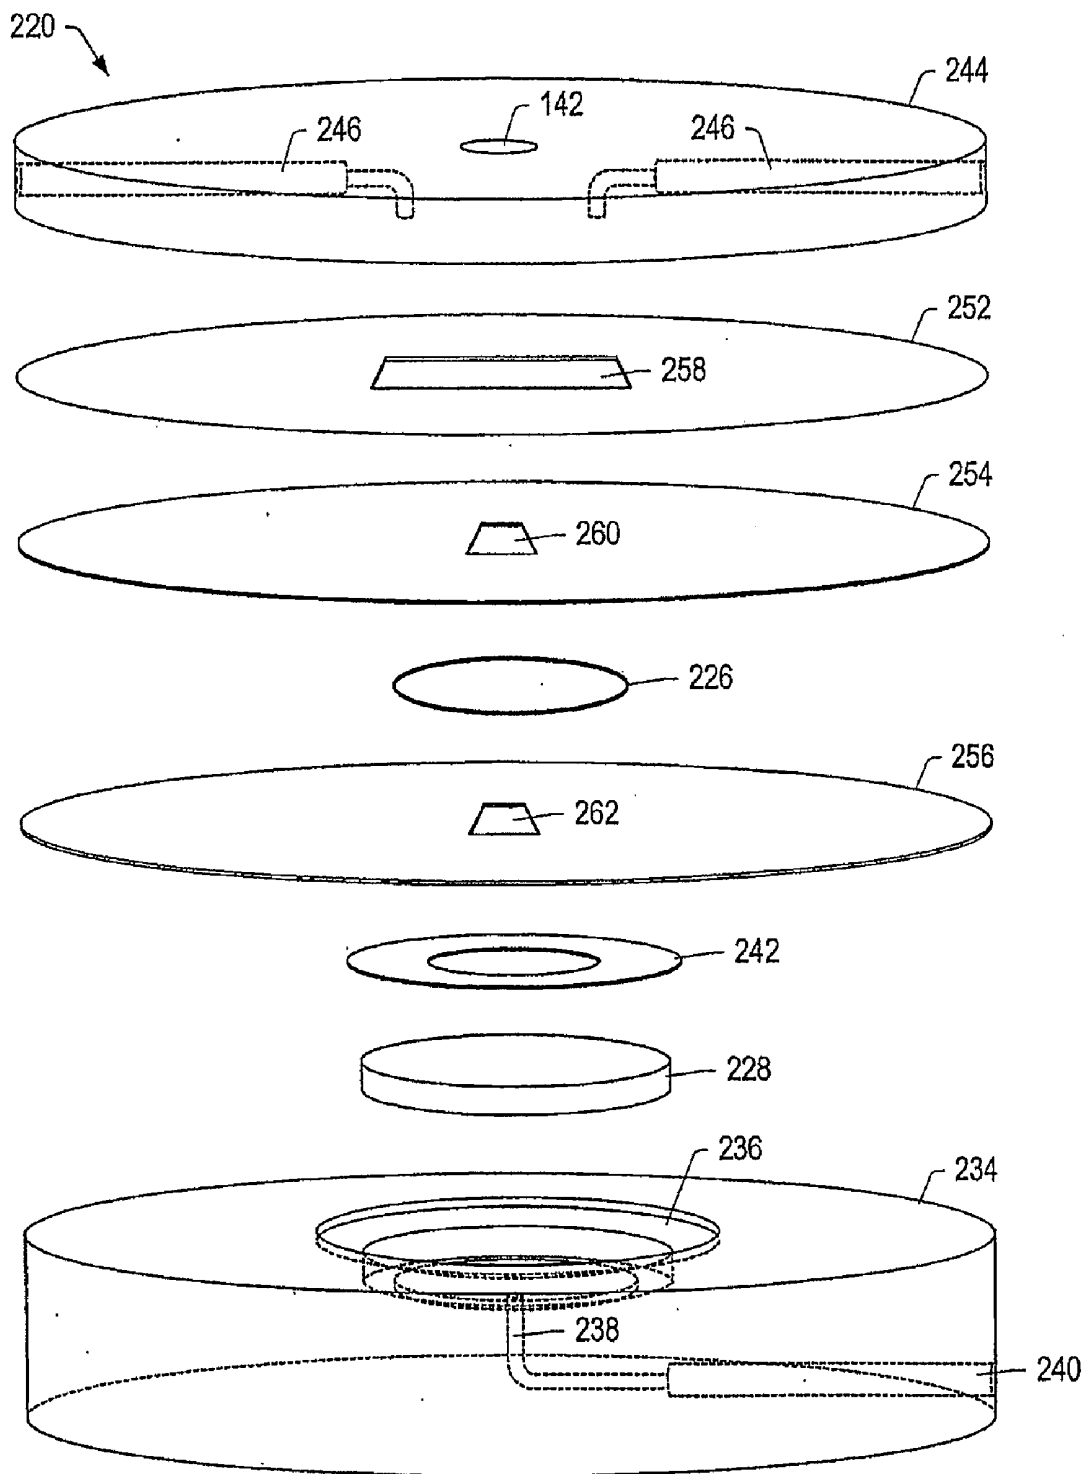


FIG. 31

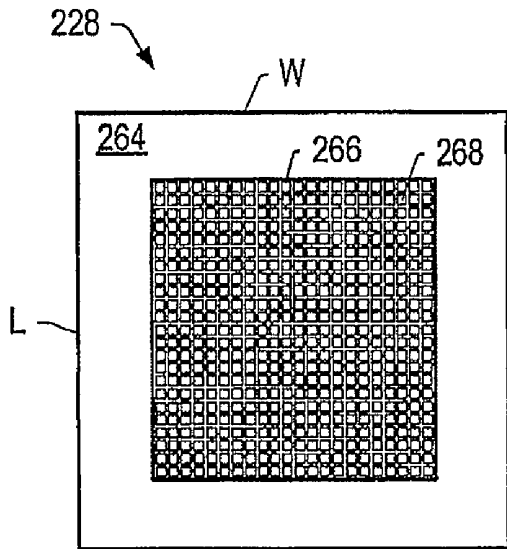


FIG. 32

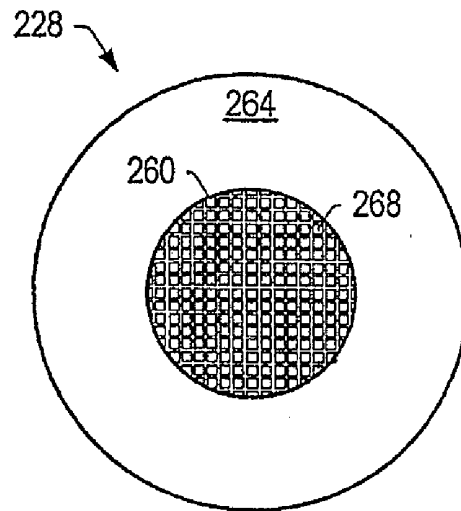


FIG. 33

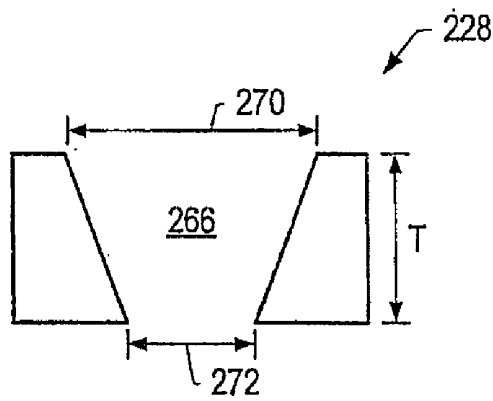


FIG. 34

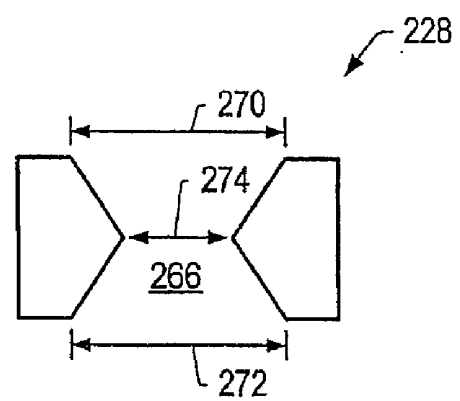


FIG. 35

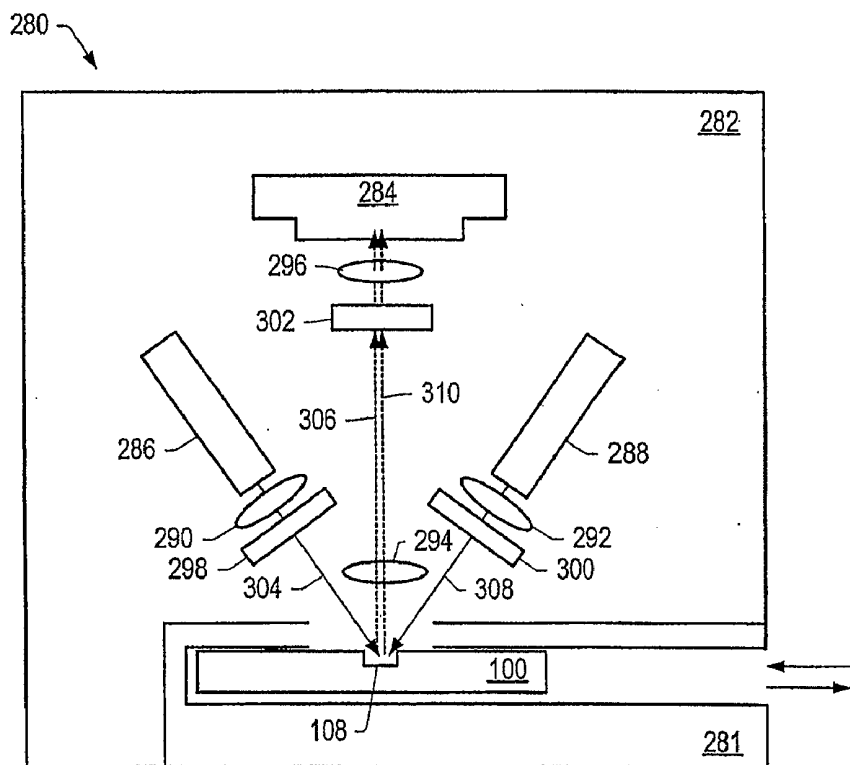


FIG. 36

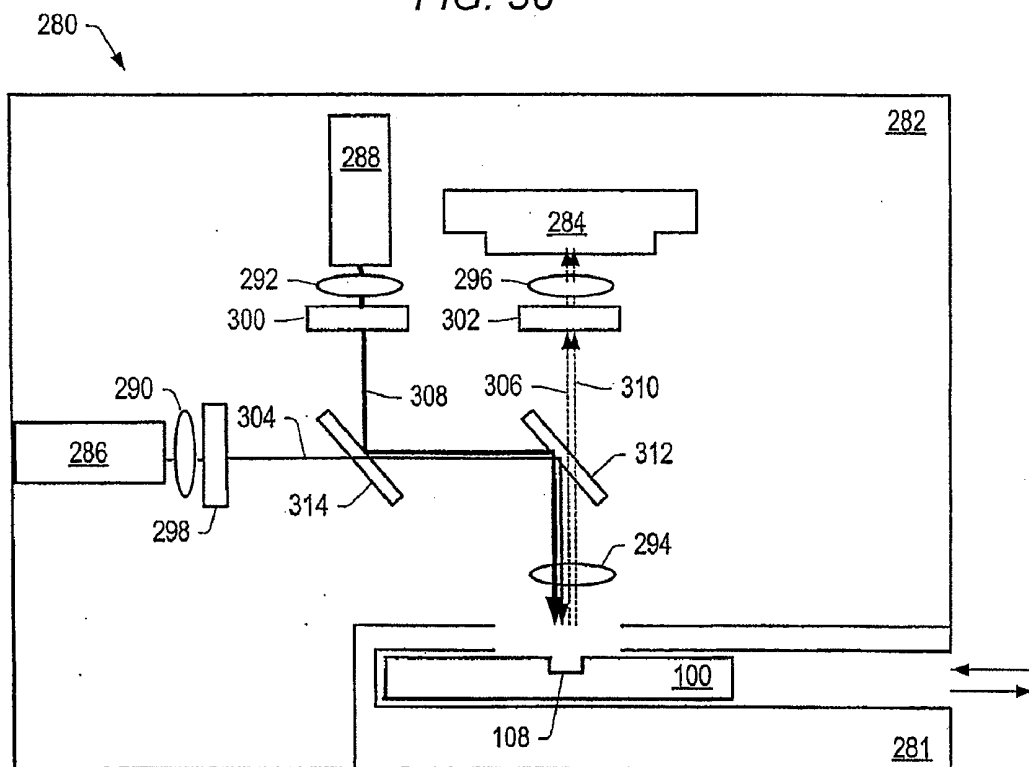


FIG. 37

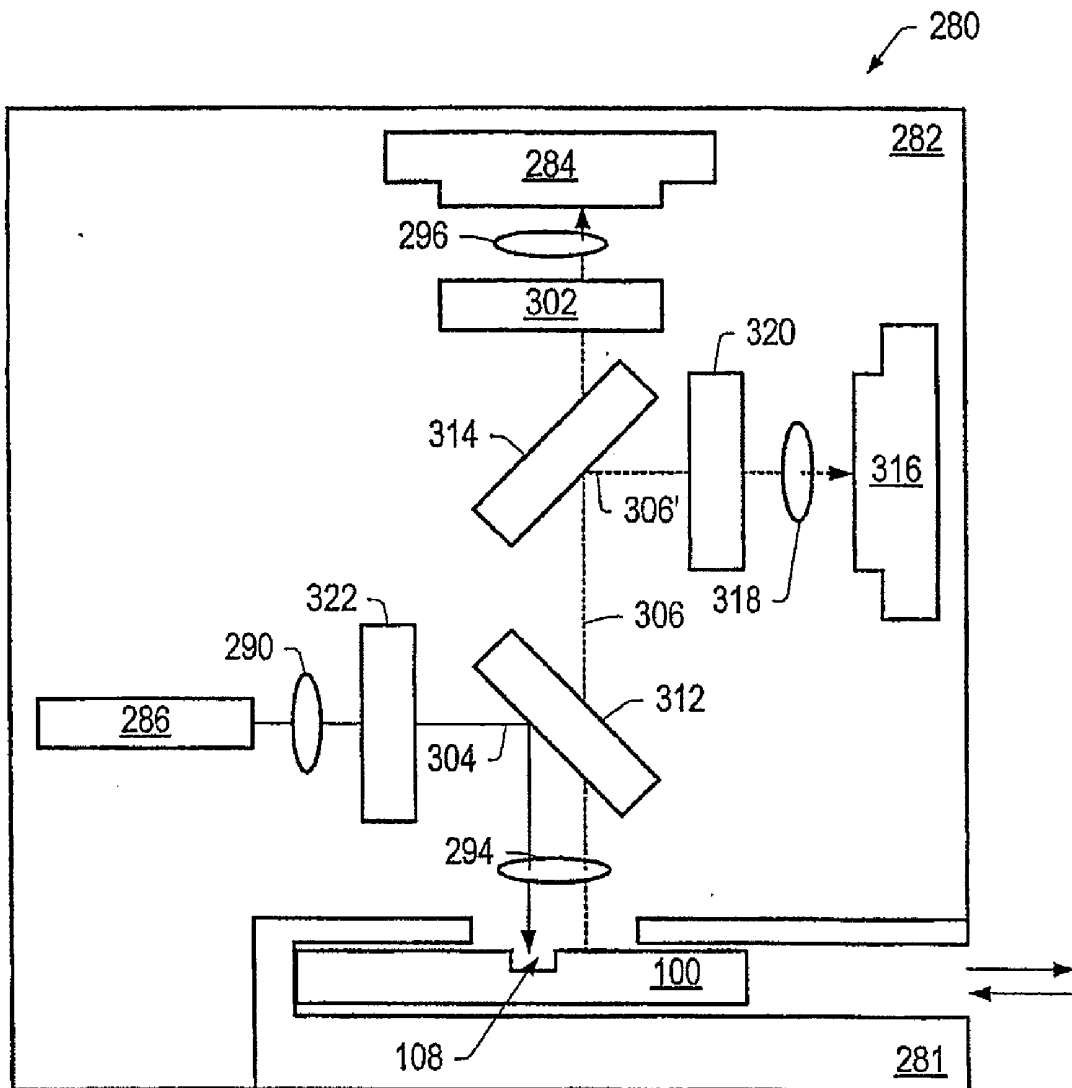


FIG. 38

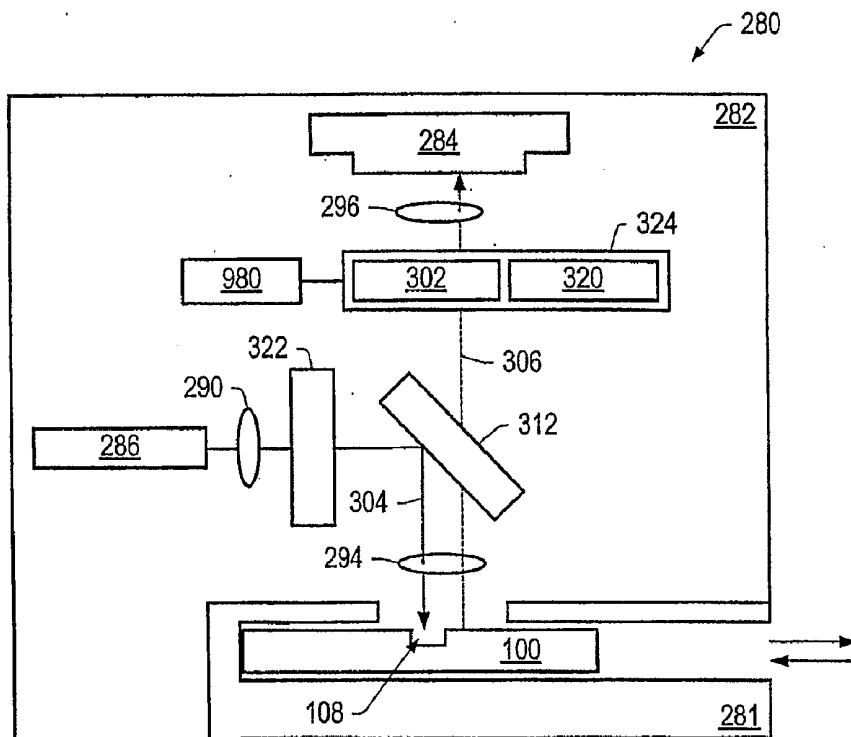


FIG. 39A

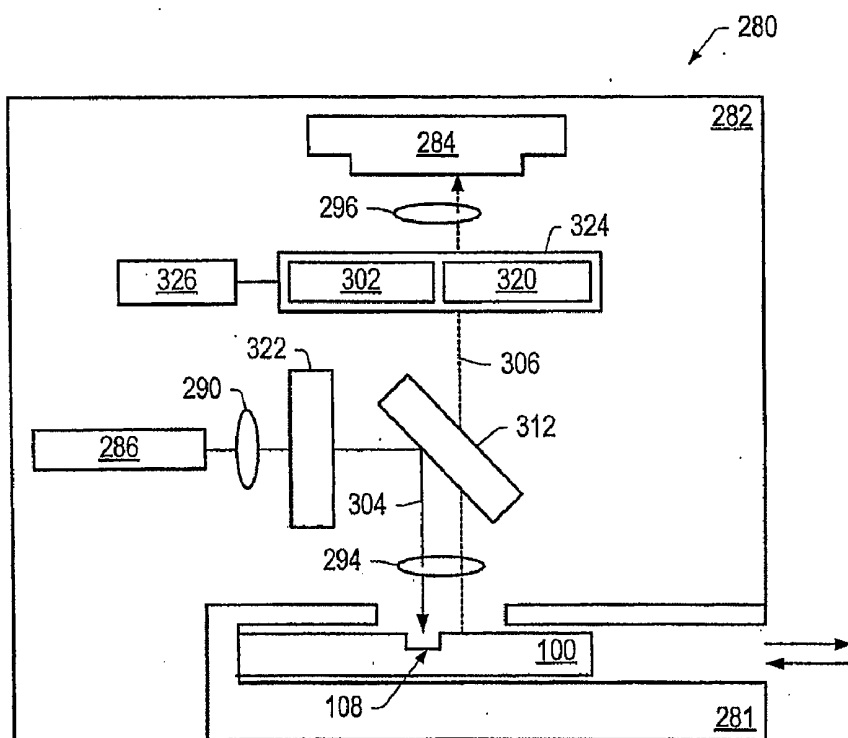


FIG. 39B

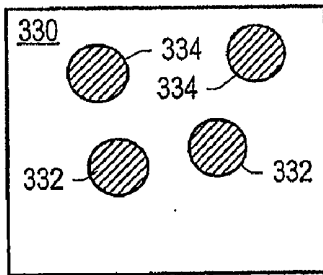


FIG. 40A

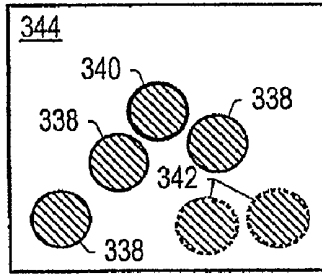


FIG. 40B

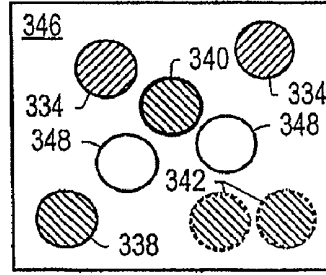


FIG. 40C

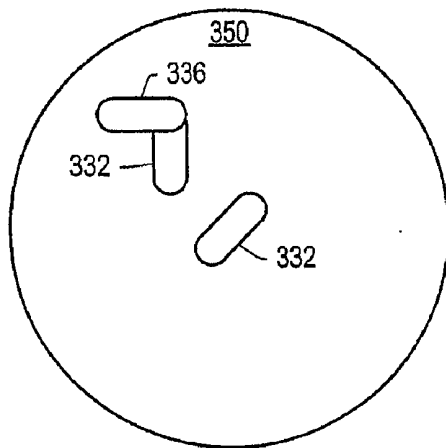


FIG. 41A

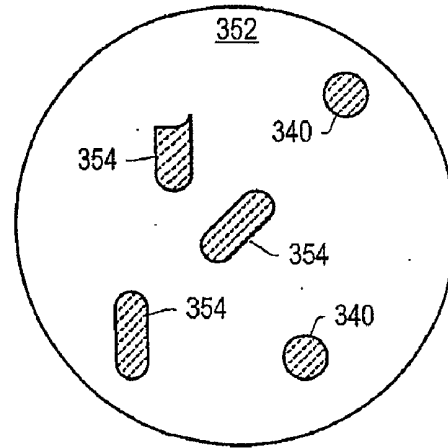


FIG. 41B

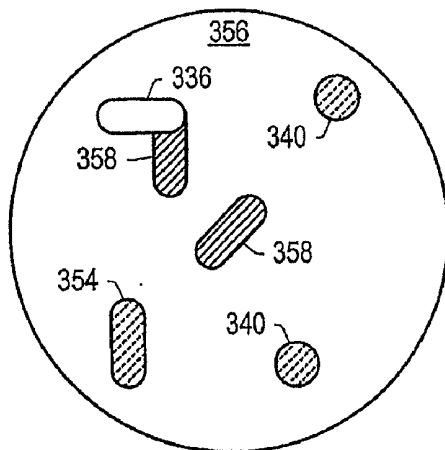


FIG. 41C

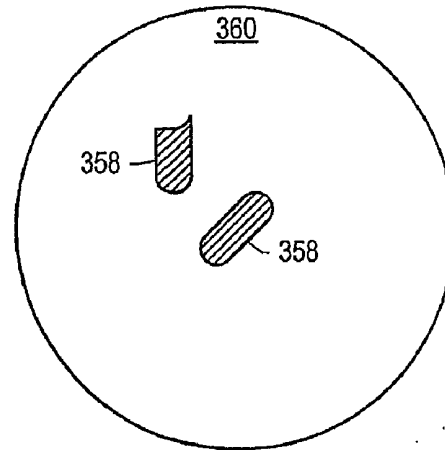


FIG. 41D

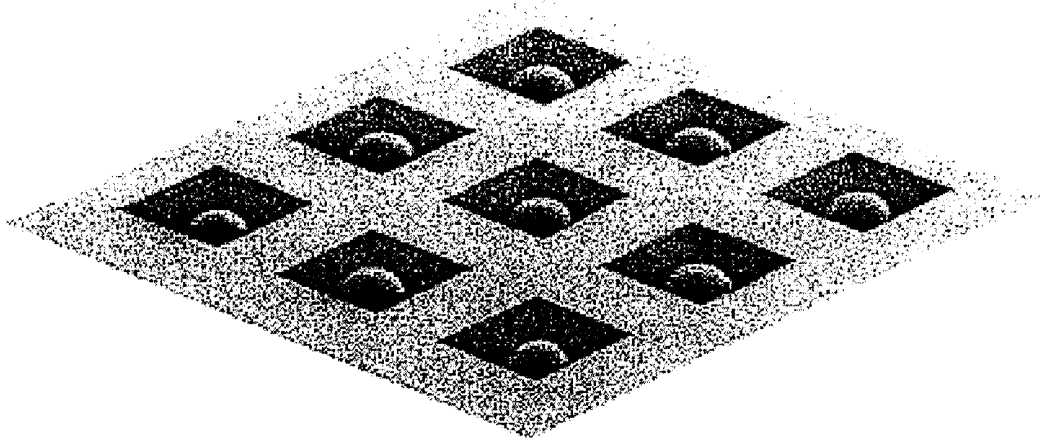


FIG. 42

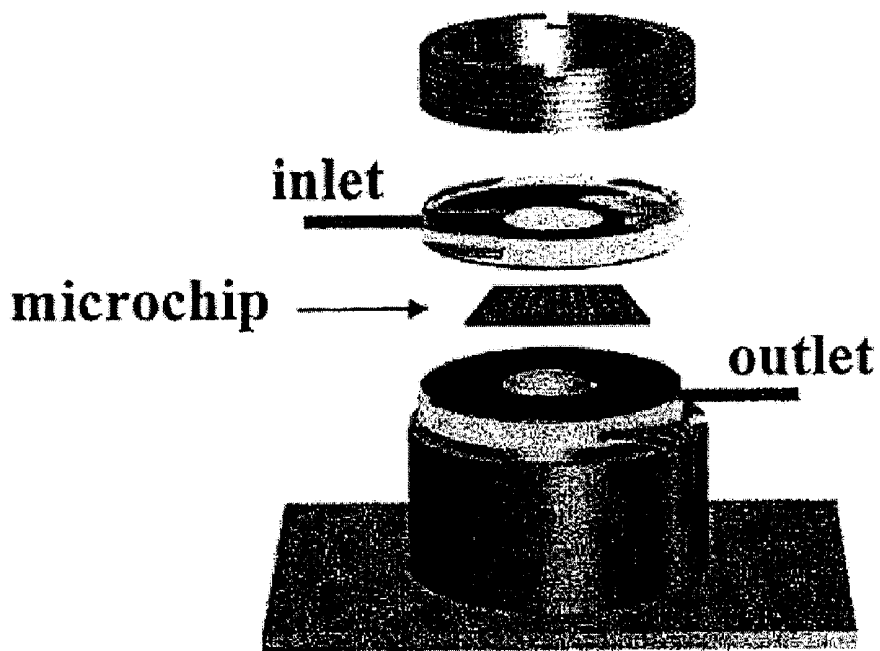


FIG. 43

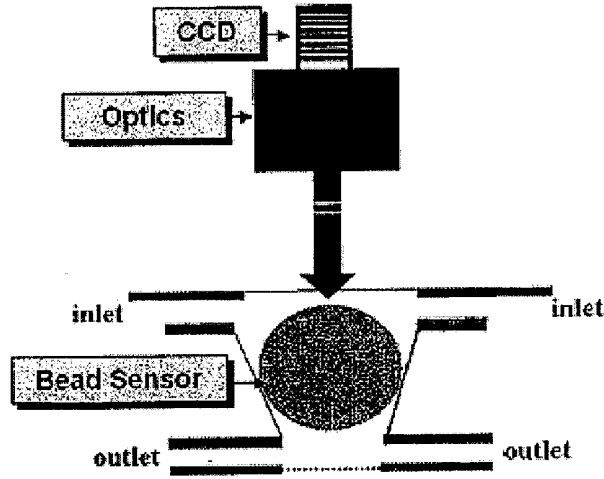


FIG. 44

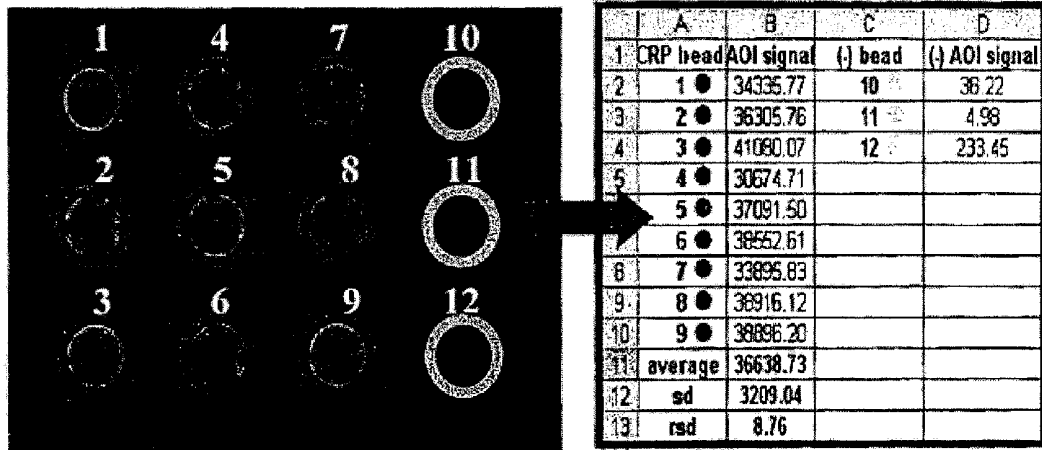


FIG. 45

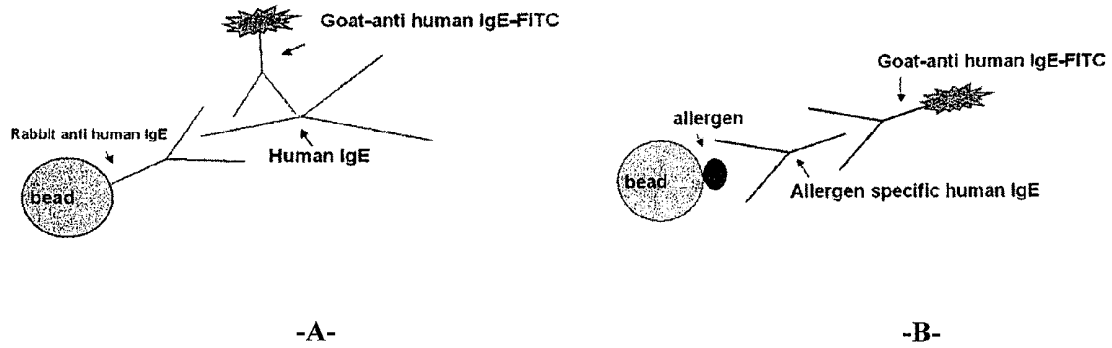


FIG. 46

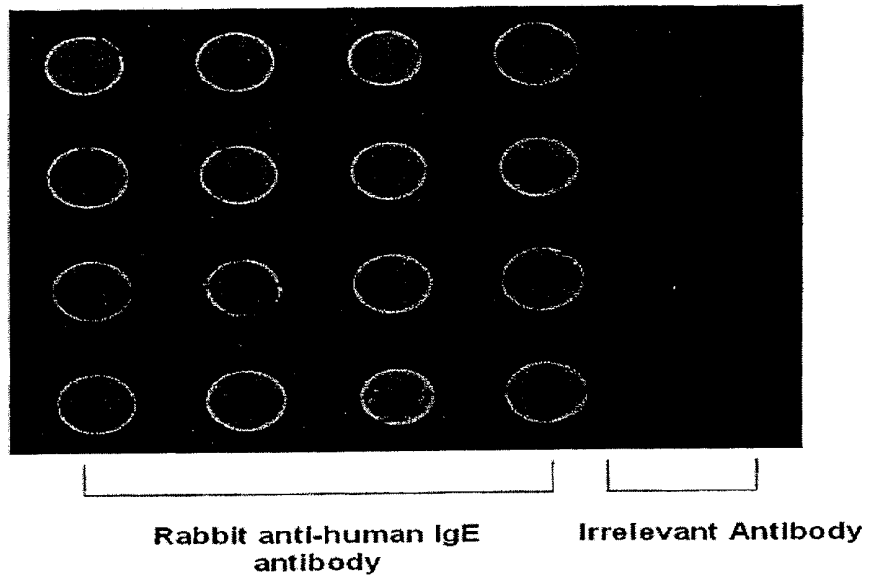


FIG. 47

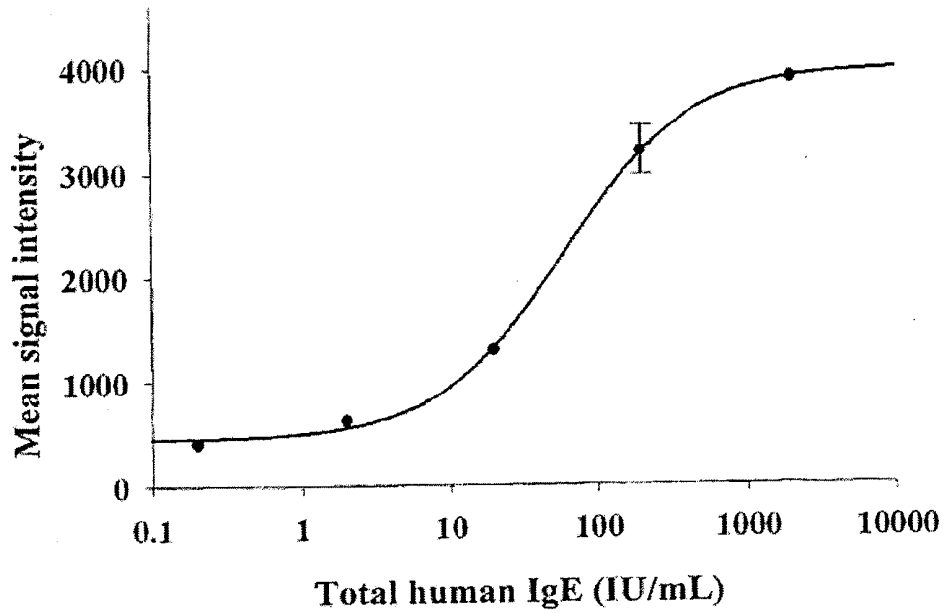


FIG. 48

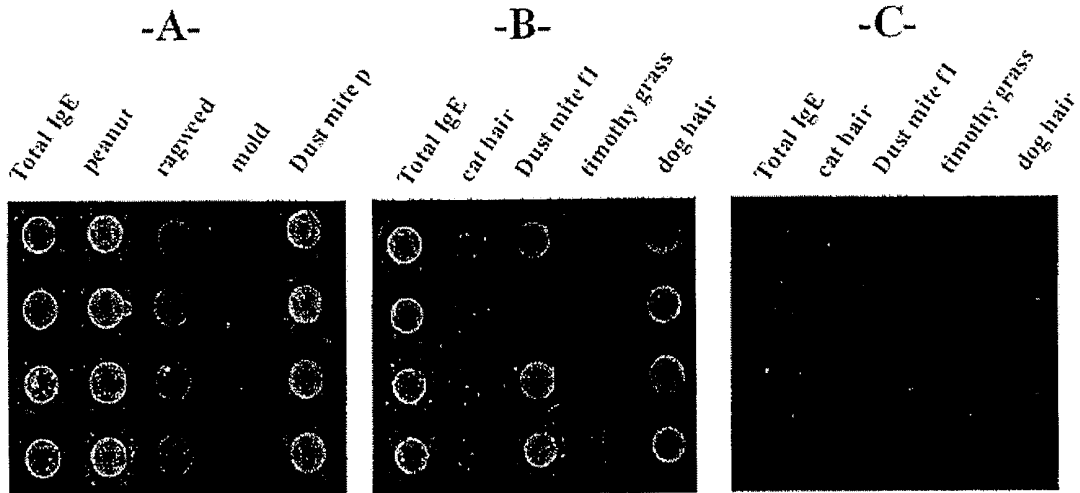


FIG. 49

DETECTING HUMAN OR ANIMAL IMMUNOGLOBIN-E

[0001] This application claims priority to U.S. Provisional Patent application Ser. No. 60/799,609 filed May 10, 2006, entitled "DETECTING HUMAN OR ANIMAL IMMUNOGLOBIN-E," which is incorporated herein by reference in its entirety.

I. FIELD OF THE INVENTION

[0002] The present invention relates to detecting human or animal immunoglobulin-E (IgE) in blood materials.

II. BACKGROUND

[0003] The development of smart sensors capable of discriminating different analytes, toxins, and bacteria has become increasingly important for clinical, environmental, health and safety, remote sensing, military, food/beverage, and/or chemical processing applications. Some sensors have been fashioned for single analyte detection. Other sensors are capable of solution phase multi-analyte detection. Latex agglutination tests ("LATs") are used to detect many different types of analytes in clinical analyses. LATs employ colloidal polymer microspheres to determine the presence (or absence) of analytes. Commercially available LATs for more than 60 analytes are used routinely for the detection of infectious diseases, illegal drugs, and pregnancies. LATs generally operate on the principle of agglutination of latex particles (e.g., colloidal polymer microspheres). LATs are set up such that agglutination occurs when antibodyderivatized latex particles become effectively "cross-linked" by a foreign antigen, resulting in the attachment of the particle to, or the inability of the particle to pass through, a filter. The cross-linked latex particles are then detected calorimetrically upon removal of the antigen carrying solution.

[0004] More recently, "taste chip" sensors have been employed that are capable of discriminating mixtures of analytes, toxins, and/or bacteria in medical, food/beverage, and environmental solutions. Certain sensors of this type are described in U.S. Patent Application Publication No. 20020197622 to McDevitt et al., which is incorporated by reference as if fully set forth herein.

[0005] According to the National Institute of Allergy and Infectious Diseases, allergies are the sixth leading cause of chronic disease in the United States. The majority of allergy sufferers are left untreated or self-treat with over-the-counter medications. The remaining are either treated symptomatically without determining the cause of the allergy or tested by skin testing. Alternatively, expensive and time-consuming in vitro tests are utilized in specialized laboratories to identify allergen-specific immunoglobulin E (IgE) in blood.

[0006] Diagnosis of allergic disease involves the combined use of a careful clinical history, physical examination, and laboratory methods for the detection of IgE antibodies of defined allergen specifications. Total IgE levels in blood have been shown to increase in patients with atopic allergic diseases such as atopic asthma, atopic dermatitis, hay fever and parasitic infestations. IgE levels may have prognostic value in assessing the risk of future allergic conditions in children. Allergen-specific IgE antibody in the serum of a patient is highly predictive of the likelihood that the individual will exhibit immediate hypersensitivity upon exposure to the

allergen. Unlike skin tests, in vitro allergen specific IgE test results are not affected by antihistamine, beta blockers and other cardiac medications, and can be used even for patients with widespread dermatopathic conditions.

[0007] Many current in vitro methodologies used to measure total and allergen-specific IgE are simply not practical for the POC setting. Most current approaches require either long and manual-intensive procedures or sophisticated instrumentation and significant amounts of sample and expensive reagents, and often extend the delay between a patient's visit to the doctor and the time of diagnosis. A more efficient multi-factorial screening approach for allergies at the POC setting is needed.

SUMMARY OF THE INVENTION

[0008] In various embodiments, systems, methods, and apparatuses to analyze one or more biological samples containing one or more analytes, in particular animal or human IgE, are described. Samples may be fluid samples. In some embodiments, an analyte-detection system is capable of analysis of a sample that includes individual analytes and mixtures of analytes. In some embodiments, the analytes include lymphocytes. The analyte-detection system may include a cartridge.

[0009] In some embodiments, the cartridge includes one or more collection regions, one or more fluid delivery systems, one or more channels, one or more reagent regions, one or more reservoirs, a detection region, or combinations thereof. The detection region may include one or more detection systems. In some embodiments, one or more collection regions, one or more detection systems, one or more fluid delivery systems, one or more channels, one or more reagent regions, and one or more reservoirs are: coupled to; at least partially positioned on; or at least partially positioned in the cartridge. In some embodiments, one or more collection regions, one or more detection systems, one or more fluid delivery systems, one or more channels, one or more reagent regions, and one or more reservoirs are at least partially contained in a body of the cartridge. In some embodiments, a body of the cartridge includes a plurality of layers coupled together.

[0010] In some embodiments, the body of the cartridge includes openings. The openings may be configured to receive one or more components used to facilitate analyte detection. One or more channels may couple the openings together. In some embodiments, one or more collection regions, one or more of the detection systems, one or more fluid packages, or combinations thereof are at least partially placed in one or more of the openings.

[0011] The collection region of a cartridge may receive a fluid and/or sample. In some embodiments, a collection region may include a cover.

[0012] Detection systems may include membrane-based detection systems and/or particle-based detection systems. The detection systems are configured to interact with at least a portion of a sample to allow detection of an analyte.

[0013] In some embodiments, a membrane of a membrane-based detection system, when one or more samples are applied to the membrane, at least partially retains desired matter in or on the membrane. In some embodiments, one or more viewing windows are optically coupled to the membrane, the viewing window being configured to allow one or more detectors to view at least a portion of the membrane.

[0014] In some embodiments, an anti-reflective material is coupled to the membrane. In some embodiments, the anti-reflective material is configured to inhibit reflection of light applied to the sample on the membrane, such that an image of at least a portion of the sample in or on the membrane is improved with respect to an image taken of the sample in the absence of the anti-reflective material.

[0015] One or more fluid delivery systems are configured to transport fluid from a first location to a second location in or on the cartridge. In some embodiments, a fluid delivery system includes one or more fluid packages and/or one or more syringes configured to facilitate transport of fluid. In some embodiments, at least one fluid delivery package is configured to create a partial vacuum, when opened, in one or more of the channels during use.

[0016] Fluid may be transported through one or more channels of the cartridge from a first location to a second location in or on the cartridge. Channels may couple one or more collection regions, one or more detection regions, and one or more fluid delivery systems to each other. In some embodiments, one or more channels are part of a fluid delivery system. In some embodiments, a shape or elevation of at least a portion of one or more of the channels is configured such that fluids flowing in or through one or more channels during use are selectively directed through the one or more channels. In some embodiments, an inside material of or on at least a portion of one or more of the channels is configured to selectively direct fluids flowing in or through one or more of the channels during use.

[0017] Valves positioned in or on one or more of the channels and/or a cartridge may control fluid flow. In some embodiments, one or more pinch valves are coupled to one or more of the channels and/or the cartridge. In some embodiments, applying pressure to one or more pinch valves positioned in or on the cartridge controls fluid flow through one or more of the channels.

[0018] One or more vents may be coupled to one or more of the channels. In some embodiments, gas is released from the cartridge through vents as fluids flow through one or more of the channels.

[0019] One or more reagent regions may include a reagent pad, at least a portion of a channel, and at least a portion of a surface of a cartridge. At least one of the reagent regions may deliver one or more reagents from the reagent region to a fluid flowing through one or more of the reagent regions during use. In some embodiments, flowing fluid through one or more reagent regions allows at least one reagent from at least one of the reagent regions to be delivered to a sample.

[0020] In some embodiments, one or more reservoirs include an overflow reservoir, a waste reservoir, or a both an overflow reservoir and a waste reservoir. The overflow reservoir and/or waste reservoir may collect excess sample or fluid. In some embodiments, a portion of fluids or samples in a cartridge is directed to an overflow reservoir of the cartridge.

[0021] In some embodiments, an analyte-detection system includes one or more cartridge-control systems. The cartridge-control systems include one or more control analytes. The cartridge-control systems may be coupled to one or more of the detection systems. One or more of the detection systems are configured to interact with at least a portion of the control analytes to allow detection of the control analyte.

[0022] A method of detecting analytes in a sample may include applying a sample on or to a collection region of a cartridge. In some embodiments, a cover is positioned over the collection region.

[0023] In some embodiments, a sample flows from a collection region to one or more detection systems, and one or more images of at least a portion the detection system are provided. In some embodiments, fluid flows through channels to and from reagent regions with the assistance of one or more fluid delivery systems. Fluids from reagent regions may flow in and/or through one or more detection systems.

[0024] A method for detection of an analyte in a sample may include applying at least a portion of a sample to a detection system of a cartridge and interacting at least a portion of the sample with the detection system to allow detection of the analyte.

[0025] A method of detecting analytes in a fluid includes applying one or more control analytes from one or more control analyte reservoirs in or on an analyte-detection cartridge to one or more detection systems in or on the analyte-detection cartridge and assessing a result from the detection system to determine whether the analyte-detection cartridge is working within a selected range.

[0026] A method for detecting lymphocytes in a sample includes applying a sample to one or more membranes in or on a cartridge and applying one or more visualization agents from one or more visualization agent locations in or on a cartridge to a least a portion of the lymphocytes retained in or on the one or more membranes.

[0027] A method for assessing CD4⁺ cells in a sample includes: applying a sample to a membrane in or on a cartridge; applying a first visualization agent to material retained on a membrane to stain any CD4⁺ cells; applying one or more additional visualization agents to the material retained on the membrane to stain any T-cells, NK-cells, and B-cells retained on the membrane; providing a first image of the CD4⁺ cells; providing a second image of the retained material; and assessing a number of CD4⁺ cells by assessing the number of stained cells in the first image that are also depicted as stained cells in the second image. In some embodiments, a ratio of CD4⁺ cells is assessed by comparing the number of stained cells that are depicted in both the first image and the second image, to the number of stained cells that are depicted in the second image.

[0028] A method of assessing CD4⁺ cells in a sample includes: applying a fluid sample to a membrane; providing a first image of material of the sample retained on the membrane; applying one or more visualization agents to the material retained on the membrane to stain at least a portion of the material retained on the membrane that does not include CD4⁺ cells; providing a second image of material retained on the membrane; assessing a number of CD4⁺ cells by assessing the number of cells that are depicted in the first image but are not depicted in the second image.

[0029] A method of analyzing a blood sample includes introducing the blood sample into an analyte-detection system, assessing a number of at least a portion of the cellular components collected by a membrane, and assessing an amount and/or identity of proteins that interact with the particle-based detection system.

[0030] An apparatus for analyzing a blood sample includes a membrane-based detection system and a particle-based detection system. The membrane-based detection system includes a membrane. The membrane collects at least a por-

tion of a first analyte in the blood sample as the blood sample passes through the membrane during use. The particle-based detection system includes one or more particles. At least a portion of the particles is configured to interact with a second analyte in the blood sample during use.

DESCRIPTION OF THE DRAWINGS

[0031] Features and advantages of the methods and apparatus of the present invention will be more fully appreciated by reference to the following detailed description of presently preferred but nonetheless illustrative embodiments in accordance with the present invention when taken in conjunction with the accompanying drawings in which:

[0032] FIG. 1 depicts a perspective view of an embodiment of a cartridge.

[0033] FIG. 2 depicts an exploded view of an embodiment of a cartridge.

[0034] FIG. 3 depicts an embodiment of a cartridge with channels.

[0035] FIG. 4 depicts an embodiment of a cartridge with fluid delivery systems with fluid packages.

[0036] FIG. 5 depicts an alternate embodiment of a cartridge.

[0037] FIG. 6 depicts a cross-sectional view of a valve.

[0038] FIG. 7 depicts a top view of an actuation system coupled to a cartridge.

[0039] FIG. 8 depicts a cross-sectional side view of an embodiment of a fluid package.

[0040] FIG. 9 depicts a top view of an embodiment of the fluid package depicted in FIG. 8.

[0041] FIG. 10 depicts a cross-sectional side view of an embodiment of a fluid package positioned in a cartridge.

[0042] FIG. 11 depicts a cross-sectional side view of rupturing the fluid package depicted in FIG. 10.

[0043] FIG. 12 depicts a cross-sectional side view of an embodiment of a fluid package in a cartridge.

[0044] FIG. 13 depicts a perspective view of a fluid delivery system that includes a fluid package and a reservoir.

[0045] FIG. 14 depicts an exploded view of the fluid delivery system depicted in FIG. 13.

[0046] FIG. 15 depicts a perspective cut-away view of the fluid delivery system depicted in FIG. 13.

[0047] FIG. 16 depicts a cut-away perspective view of the bottom of the fluid delivery system depicted in FIG. 13.

[0048] FIG. 17 depicts a top view of a seal offset from a top layer opening of the fluid delivery system depicted in FIG. 13.

[0049] FIG. 18 depicts a perspective view of an alternate embodiment of a fluid delivery system.

[0050] FIG. 19 depicts an exploded view of the fluid delivery system depicted in FIG. 18.

[0051] FIG. 20 depicts an embodiment of a fluid package used in the fluid delivery system depicted in FIGS. 18 and 19.

[0052] FIG. 21 depicts an exploded view of an alternate embodiment of a fluid delivery system.

[0053] FIGS. 22A and 22B depict embodiments of fluid packages.

[0054] FIG. 23 depicts an embodiment of a fluid bulb for fluid delivery.

[0055] FIG. 24 depicts an alternate embodiment of fluid bulb for fluid delivery.

[0056] FIGS. 25A-25H depict embodiments of syringes.

[0057] FIGS. 26A-26B depict an embodiment of syringes coupled to a cartridge. FIG. 26B depicts a magnified view of a portion of the cartridge depicted in FIG. 26A.

[0058] FIG. 27 depicts an embodiment of a cartridge that includes more than one detection system.

[0059] FIG. 28 depicts a top view of an embodiment of a multi-functional cartridge.

[0060] FIG. 29 depicts an exploded view of the multi-functional cartridge depicted in FIG. 28.

[0061] FIG. 30 depicts an exploded view of a membrane-based detection system.

[0062] FIG. 31 depicts an exploded view of a membrane-based detection system with directed fluid flow.

[0063] FIG. 32 depicts a top view of a membrane support with a parallelogram shape.

[0064] FIG. 33 depicts a top view of a membrane support with a euclidian shape.

[0065] FIG. 34 depicts a cross-sectional view of an embodiment of an open area of a membrane support.

[0066] FIG. 35 depicts a cross-sectional view of an alternate embodiment of an open area of a membrane support.

[0067] FIG. 36 depicts a schematic diagram of a cartridge positioned in an optical platform with two light sources.

[0068] FIG. 37 depicts a schematic diagram of a cartridge positioned in an alternate optical platform with two light sources.

[0069] FIG. 38 depicts a schematic diagram of a cartridge positioned in an optical platform with a single light source.

[0070] FIGS. 39A-39B depict schematic diagrams of a cartridge positioned in an optical platform that includes movable filters.

[0071] FIGS. 40A-40C depict representations of images of cells obtained using an analyte-detection system.

[0072] FIGS. 41A-41D depict representations of images of cells obtained using an analyte-detection system.

[0073] FIG. 42 further illustrates the method and apparatus as applied to the detection of IgE.

[0074] FIG. 43 further illustrates the method and apparatus as applied to the detection of IgE.

[0075] FIG. 44 further illustrates the method and apparatus as applied to the detection of IgE.

[0076] FIG. 45 further illustrates the method and apparatus as applied to the detection of IgE.

[0077] FIG. 46 further illustrates the method and apparatus as applied to the detection of IgE.

[0078] FIG. 47 further illustrates the method and apparatus as applied to the detection of IgE.

[0079] FIG. 48 further illustrates the method and apparatus as applied to the detection of IgE.

[0080] FIG. 49 further illustrates the method and apparatus as applied to the detection of IgE.

[0081] FIG. 50 further illustrates the method and apparatus as applied to the detection of IgE.

[0082] FIG. 51 further illustrates the method and apparatus as applied to the detection of IgE.

DETAILED DESCRIPTION OF THE INVENTION

[0083] In various embodiments, an analyte-detection system may be used to analyze a sample containing one or more analytes. Samples may be fluid samples, e.g., a liquid sample or a gaseous sample. The analyte-detection system may, in some embodiments, generate patterns that are diagnostic for both the individual analytes and mixtures of the analytes. In some embodiments, the analyte-detection system includes a membrane capable of retaining a portion of the sample. The analyte-detection system, in certain embodiments, may include a plurality of chemically sensitive particles, formed in

an ordered array, capable of simultaneously detecting different analytes. In some embodiments, the analyte-detection system may be formed using a microfabrication process, thus allowing the analyte-detection system to be economically manufactured.

[0084] Terms used herein are as follows:

[0085] "Analyte" refers one or more substances undergoing analysis. Examples of analytes include, but are not limited to, organic molecules, inorganic molecules, cells, bacteria, viruses, fungi, and parasites.

[0086] "Anti-reflective" refers to inhibiting the reflection of light at predetermined wavelengths.

[0087] "Cartridge" refers to a removable unit designed to be placed in a larger unit.

[0088] "Couple" refers to either a direct connection or an indirect connection (e.g., one or more intervening connections) between one or more objects or components.

[0089] "CRP" refers to C-reactive protein.

[0090] "Detection system" refers to one or more systems designed to interact with one or more analytes during use.

[0091] "Detector" refers to one or more devices capable of detecting the presence of one or more analytes, one or more signals produced by one or more of the analytes, one or more signals produced by the interaction of one or more analytes with a detection system, or combinations thereof. Signals produced by analytes include, but are not limited to, spectroscopic signals. Spectroscopic signals include, but are not limited to, signals produced at wavelengths detectable in an ultraviolet ("UV") region, a visible region and an infrared ("IR") region of the electromagnetic spectrum. Spectroscopic signals also include signals produced by fluorescence of an analyte or a component of a detection system. The detector may be, but is not limited to an optical digital camera, a charge-coupled-device ("CCD"), a complementary-metal-oxide-semiconductor ("CMOS") detector, or a spectrophotometer capable of detecting UV, visible and/or IR wavelengths of light.

[0092] "Fluid" refers to a substance in a gas phase or a liquid phase.

[0093] "Fluid delivery system" refers to one or more systems or devices capable of causing a fluid to flow. A fluid delivery system may include a plurality of components. Components that may be part of a fluid delivery system include, but are not limited to, reservoirs containing fluids, flexible chambers containing fluids, channels, reagent reservoirs, buffer reservoirs, fluid packages, syringes, fluid bulbs, and/or pipettes.

[0094] "Fluid package" refers to a pouch, a container, or a chamber configured to contain one or more fluids.

[0095] "Fluorophore" refers to one or more fluorescent molecules or compounds.

[0096] "Hydrophilic material" refers to one or more materials having the ability to hydrogen bond with water. Hydrophilic materials may have an affinity for aqueous solutions.

[0097] "Hydrophobic material" refers to one or more materials ineffective at hydrogen bonding with water. Hydrophobic materials may lack an affinity for water.

[0098] "LED" refers to light emitting diode.

[0099] "Membrane" refers to one or more thin sheets or layers capable of retaining matter from a fluid and/or a sample.

[0100] "Positioned in" or "positioned on" refers to placing one or more substances at least partially or fully in or on an opening or a surface of a substrate.

[0101] "RBCs" refer to red blood cells.

[0102] To "stain" refers to applying one or more compounds to a substance to alter the absorbance and/or fluorescence of the substance.

[0103] "Visualization agent" refers to one or more compounds capable of altering an appearance of a material. Visualization agents may, in some embodiments, stain a material.

[0104] "WBCs" refer to white blood cells.

[0105] Analytes in a sample may be analyzed using an analyte-detection system. In some embodiments, a sample is a bodily fluid (e.g., saliva, urine, and/or blood). The blood sample may be human blood or mammalian blood. A blood sample may be obtained from any species. Collection of a sample may be accomplished by making an incision (e.g., a prick or cut) in a part of (e.g., a finger) a human body to allow collection of the sample (e.g., blood).

[0106] The sample may be collected with a tube, a fluid bulb, a syringe, or a pipette. The sample may be directly transferred to a cartridge of the analyte-detection system (e.g., transfer to a collection region of the cartridge) using the fluid bulb, the syringe, or the pipette. For example, a sample is collected in a tube or a vacuum tube and transferred to a collection region of the cartridge. In some embodiments, a cartridge may include a conduit coupled to a disposable tip. The disposable tip may puncture a portion of a human body and draw a sample into the cartridge. In some embodiments, a sample is reacted with one or more reagents and/or one or more visualization agents in a sample collection device prior to being transferred to the cartridge.

[0107] The sample may be diluted before it is applied to a cartridge or after it is applied to the cartridge. For example, a sample of human blood may be diluted before applying it to a collection region of a cartridge. The use of a sample collection device may limit health and safety risks associated with exposure to pathogens present in a sample. Using a sample collection device, may allow a sample to be directly transported from the source to the instrument without further handling.

[0108] Sample collection devices are described by McDevitt et al., in U.S. patent application Ser. Nos. 11/022,176 entitled "INTEGRATION OF FLUIDS AND REAGENTS INTO SELF-CONTAINED CARTRIDGES CONTAINING SENSOR ELEMENTS"; 11/020,443 entitled "INTEGRATION OF FLUIDS AND REAGENTS INTO SELF-CONTAINED CARTRIDGES CONTAINING SENSOR ELEMENTS"; 11/020,442 entitled "INTEGRATION OF FLUIDS AND REAGENTS INTO SELF-CONTAINED CARTRIDGES CONTAINING SENSOR ELEMENTS"; 11/022,365 "INTEGRATION OF FLUIDS AND REAGENTS INTO SELF-CONTAINED CARTRIDGES CONTAINING SENSOR ELEMENTS"; 11/021,123 entitled "PARTICLE ON MEMBRANE ASSAY SYSTEM"; and 11/022,219 entitled "MEMBRANE ASSAY SYSTEM INCLUDING PRELOADED PARTICLES", all of which were filed on Dec. 22, 2004 and are herein incorporated by reference.

[0109] The analyte-detection system may include, but is not limited to, one or more apparatuses (e.g., cartridges), an optical platform, one or more detectors, an analyzer, or combinations thereof. The cartridge may include, but is not limited to, one or more sample collection devices, one or more collection regions, one or more fluid delivery systems, one or more reagent regions, one or more detection regions, or combinations thereof. The detection regions may include one or more detection systems. The optical platform may include,

but is not limited to, one or more detectors, one or more light sources, one or more lenses, one or more filters, one or more dichroic mirrors, one or more shutters, one or more actuators, or combinations thereof. The analyzer may include one or more computer systems and/or one or more microscopes. In some embodiments, the analyte-detection system includes a housing. The housing may include the optical platform and/or one or more cartridges.

[0110] In some embodiments, a cartridge is self-contained and/or disposable. The cartridge may include all reagents and/or fluids necessary for the detection of one or more analytes in a sample. Use of a self-contained and/or disposable cartridge may limit environmental and health risks associated with handling of fluids and/or samples.

[0111] In some embodiments, one or more barcodes or other readable indicia are positioned on a cartridge. A detector and/or an analyzer of the analyte-detection system may read the barcode to determine hardware and/or software specifications for the assay. Using barcodes or other readable indicia may allow a user to analyze a plurality of cartridges using the same analyte-detection system. When the cartridge is positioned in an analyte-detection system, a reader in the analyte-detection system may read the indicia on the cartridge and set the system specifications for the indicated test. A bar code or indicia may represent information such as, but not limited to, the type of analyte to be detected, light sources which should be used, process time, sample number or code, detector settings, or combinations thereof. System specifications include, but are not limited to: which light sources, filters, or lenses to use; detector settings; fluid delivery system activation order and/or times; actuator activation sequence; actuator positions; exposure times; sample incubation time; and/or which visualization agents are used in the cartridge.

[0112] A cartridge may include indicia that tell a user which direction to insert the cartridge into the analyte-detection system. For example, a body of a cartridge may include a notch, arrow and/or a barcode to indicate the proper placement of the cartridge.

[0113] In some embodiments, a cartridge includes a viability indicator (e.g., a temperature indicator). A viability indicator may indicate if the cartridge has been exposed to conditions that could damage the cartridge and/or one or more chemical components of the cartridge. For example, a temperature-based indicator indicates if the cartridge has been exposed to temperatures that are above or below a temperature that would cause decomposition of one or more chemical components in the cartridge. An analyte-detection system may read the viability indicator to determine if the cartridge is viable prior to initiating any detection operations with the cartridge.

[0114] The cartridge may be formed of an inert and/or biodegradable material. The cartridge may be sized to allow the cartridge to be hand-held and/or portable. In some embodiments, a cartridge has dimensions, which allows the cartridge to be inserted into a housing of an analyte-detection system.

[0115] In some embodiments, a cartridge body is substantially planar. A width (w) of the cartridge may range from about 30 mm to about 100 mm, from about 40 mm to about 90 mm, from about 50 mm to about 80 mm, or from about 60 mm to about 70 mm. A length (l) of the cartridge may range from about 50 mm to about 300 mm, 60 mm to about 200 mm, 70 mm to about 150 mm, or from about 80 mm to about 100 mm. A height (h) of the cartridge may range from about 1 mm to

about 30 mm, from about 5 mm to 20 mm, or from about 10 mm to 15 mm. In some embodiments, a cartridge is about 35 mm wide and 125 mm long, about 35 mm wide and about 75 mm long, or about 50 mm wide and about 75 mm long.

[0116] A cartridge body may include one or more openings designed to receive one or more components used to facilitate analyte detection. Components include, but are not limited to, a collection region (e.g., a sample collection pad), a fluid delivery system (e.g., a fluid package, a fluid bulb, a syringe, and/or a fluid reservoir), reservoirs, a membrane-based detection system, a particle-based detection system, or combinations thereof. Components may be positioned in one or more cartridge body openings. Adhesive may be used to secure the components to the cartridge body and/or within the openings formed in the cartridge body. Openings may be designed to receive a specific component. For example, an opening designed for a collection region may have a specific shape that is different than an opening designed for a fluid delivery system component. In some embodiments, openings for components have the same dimensions and/or shape. In some embodiments, a cartridge body includes channels coupling one or more of the openings in or on the cartridge together. The ability to customize the cartridge body may allow many different configurations of a cartridge to be produced.

[0117] In some embodiments, collection regions, fluid delivery systems, reagent regions, and/or detection systems may be coupled to the cartridge, directly attached to the cartridge, positioned in the cartridge, or positioned on the cartridge. Collection regions, reagent regions, fluid delivery systems, and/or detection systems may be incorporated in a cartridge body. Collection regions, reagent regions, fluid delivery systems, and detection systems may be at least partially contained in a cartridge body.

[0118] In some embodiments, components are at least partially positioned in different layers of a body of the cartridge. For example, the collection region may be positioned in a different layer of the cartridge than the detection system. In some embodiments, reservoirs (e.g., sample collection reservoir, overflow reservoir, and/or waste reservoir) are positioned in the same layer or in more than one layer. For example, a waste reservoir is positioned in a different layer of the cartridge than the detection system and/or the collection region. Fluid delivery systems may be positioned in one or more of the same layers of the cartridge body. The cartridge body may include one or more layers that retain fluid in at least a portion of the cartridge. In some embodiments, a top layer includes an opening coupled to the sample collection region to allow application of the sample to the sample collection region, while retaining fluid in other portions of the cartridge.

[0119] In certain embodiments, a cartridge with one or more openings has a variety of configurations. For example, a cartridge includes a detection region and one or more openings. A collection region, one or more fluid delivery systems and/or one or more reservoirs may be positioned in the openings of the cartridge. Alternatively, a cartridge includes a sample collection region and one or more openings. A detection system and/or at least one fluid package may be positioned in the openings. In another example, a cartridge includes one or more fluid delivery systems and one or more openings. Components (e.g., a sample collection region and/or detection system) may be inserted the openings.

[0120] The collection region of a cartridge may be coupled to, positioned in, or positioned on the cartridge. The collec-

tion region may collect sample from a sample collection device. In some embodiments, fluids other than sample are collected in the collection region.

[0121] The collection region may include a channel positioned at a predetermined height with respect to the region. When a sample is deposited in the collection region, any sample excess sample will flow through the channel into an overflow reservoir and/or waste reservoir of the cartridge. The height at which the channel is positioned with respect to the region will determine the amount of sample that is collected in the collection region. Inclusion of the channel may inhibit sample from spilling out of a collection region. Inhibiting a sample from overflowing from the collection region may lessen exposure to potentially hazardous material. In some embodiments, a collection region of a cartridge includes and/or is a sample collection reservoir and/or a collection pad.

[0122] One or more fluid delivery systems may be coupled to, positioned in, positioned on, or embedded in a cartridge. In some embodiments, fluid delivery systems containing appropriate reagents, buffers, and/or visualization agents are positioned in openings in the cartridge body. Some fluid delivery systems are described in U.S. Pat. Nos. 5,096,660 to Lauks et al.; 5,837,199 to Dumschat; and 6,010,463 to Lauks et al., all of which are hereby incorporated by reference. In some embodiments, gravity, elevation changes within the cartridge and/or channel, capillary forces, or combinations thereof, promotes and/or facilitates the transport of fluids in the cartridge. In certain embodiments, pumps and/or vacuums are coupled to the cartridge, in addition to fluid delivery systems, to assist fluid flow.

[0123] A cartridge may include one or more reagent regions. One or more reagent regions may be at least partially coupled to, positioned on, or positioned in the cartridge. In some embodiments, a reagent region includes one or more reagents, visualization agents, and/or buffers that are disposed on one or more reagent pads, one or more surfaces of a channel, one or more surfaces of a cartridge, or a combination of these locations.

[0124] The reagents, visualization agents, and/or buffers may be in solid, liquid, or gaseous state. In some embodiments, a reagent region includes one or more reagents, visualization agents, and/or buffers entrained in a dissolvable material. When a fluid contacts (e.g., passes over) the dissolvable material, at least a portion of the reagents, visualization agents, and/or buffers entrained in the dissolvable material may be released. For example, dried reagents may be positioned in or on a dissolvable material. Fluid passing over the dissolvable material may at least partially dissolve the dissolvable material and partially reconstitute the dried reagents.

[0125] A reagent pad of a reagent region may be, but is not limited to, a filter, absorbent pad, or container. Reagents including, but not limited to, visualization agents, anti-coagulants, and/or particles may be positioned in the reagent pad and/or on a surface of the reagent pad such that fluid passing over and/or through the reagent pad may at least partially reconstitute the reagents contained in or on the pad. In some embodiments, a reagent pad performs as a filter to remove large particles from a fluid flowing through the reagent pad.

[0126] In certain embodiments, dried reagents, lyophilized reagents, and/or solid reagents are positioned in or coated on a surface of a reagent region (e.g., surfaces of a channel or a cartridge). As fluid passes through the channel, reagents and/or visualization agents may be reconstituted. Dried, lyophilized, or solid reagents may be more stable. Using

reagents that are dried, lyophilized, or are in a solid state may increase the shelf life of a cartridge. Using dried, lyophilized, or solid reagents may allow a cartridge to be stored at ambient temperatures rather than in a controlled temperature storage unit (e.g., a refrigerator).

[0127] In some embodiments, one or more reservoirs (e.g., one or more overflow reservoirs and/or one or more waste reservoirs) are coupled to, positioned in, or positioned on a cartridge. The overflow reservoir and/or waste reservoir may collect excess fluid (e.g., excess sample, excess visualization agent, and/or excess reagents).

[0128] The overflow reservoir is, in some embodiments, coupled to a collection region, a detection region, a detection system, and/or one or more reagent regions. The overflow reservoir may be coupled to the collection region to allow an excess amount of sample (e.g., an amount of sample greater than a predetermined amount of sample) applied to the collection region to flow to the overflow reservoir. Coupling the overflow reservoir to the collection region may allow a predetermined amount of sample to be collected. Coupling the overflow reservoir to the collection region may inhibit overfilling the collection region. Inhibiting overfilling of the collection region may inhibit release of potentially hazardous material.

[0129] In some embodiments, the overflow reservoir is coupled to the detection region and/or detection system to inhibit excess fluid from entering the detection region and/or detection system. If excess fluid enters the detection region and/or detection system, it may disturb matter and/or particles retained in or on the detection region and/or detection system. Disturbance of retained matter and/or particles may cause the matter and/or the particles to leave the detection region and/or detection system. For example, if too much fluid flows onto a membrane positioned in or on a detection region and/or a detection system, matter retained on a surface of the membrane may be disturbed and a portion of the retained matter may flow into proximate channels or regions before analysis.

[0130] One or more detection regions of a cartridge include areas of the cartridge where one or more detection systems are located. Detection systems may be coupled to, positioned in, or positioned on, a cartridge. It should be understood, that various combinations of detection systems in, on, or coupled to the cartridge are possible. For example, one detection system may be positioned in an opening of the cartridge, while another detection system is positioned on the cartridge. A detection system may be coupled to the cartridge, while another detection system is positioned in the cartridge. Detection systems may include, but are not limited to, a membrane-based detection system and/or a particle-based detection system. A detection system is selected based on the analyte of interest. For example, a membrane-based detection system may be selected to assess cells or bacteria in a fluid and/or sample.

[0131] Detection systems and methods of using the detection systems are described herein and in U.S. patent application Ser. Nos. 11/020,442; 11/022,365; 11/021,123; and 11/022,219, and in the following U.S. patents, U.S. Published patent applications, and patent applications to McDevitt et al., which are hereby incorporated by reference: U.S. Pat. Nos. 6,908,770; 6,680,206; 6,602,702; 6,589,779; 6,649,403; and 6,713,298; U.S. Patent Application Publication Nos. 20020160363; 20040029259; 20030064422; 20030186228; 20040053322; 20050136548; 20050164320; 20050214863; U.S. patent application Ser. Nos. 09/616,731 entitled

“METHOD AND APPARATUS FOR THE DELIVERY OF SAMPLES TO A CHEMICAL SENSOR ARRAY” filed Jul. 14, 2000; 10/522,499 entitled “CAPTURE AND DETECTION OF MICROBES BY MEMBRANE METHODS” filed Jan. 24, 2005; 10/470,646 entitled “CAPTURE AND DETECTION OF MICROBES BY MEMBRANE METHODS” filed Jan. 24, 2005; 10/522,926 entitled “CAPTURE AND DETECTION OF MICROBES BY MEMBRANE METHODS” filed Jan. 24, 2005; 10/544,864 entitled “MICROCHIP-BASED SYSTEM FOR HIV DIAGNOSTICS” filed Aug. 5, 2005; and 10/544,954 entitled “MULTI-SHELL MICROSPHERES WITH INTEGRATED CHROMATOGRAPHIC AND DETECTION LAYERS FOR USE IN ARRAY SENSORS” filed on Aug. 8, 2005.

[0132] FIG. 1 depicts a perspective top view of an embodiment of a cartridge. Cartridge **100** includes collection region **102**, cover **104**, fluid channel **106**, and detection region **108**. A sample may be placed in collection region **102**. In some embodiments, other fluids (e.g., reagents and/or buffer solutions) may be added to the collection region and mixed with the sample. The sample may flow from collection region **102** through channel **106** to detection region **108**.

[0133] Collection region **102** may include, but is not limited to, a reservoir, a pad, a channel, a capillary, a tube, a vacuum collection tube (e.g., a Vacutainer® commercially available from Becton, Dickinson Company Franklin Parks, N.J., USA), an opening in the cartridge, or combinations thereof. In some embodiments, collection region **102** is a portion of the detection system on which sample is applied. In certain embodiments, collection region **102** is a membrane.

[0134] In some embodiments, cover **104** is removable. Cover **104** may cover a portion or all of collection region **102**. The use of cover **104** is optional. Cover **104** may be positioned manually or automatically. In some embodiments, an analyte-detection system automatically positions the cover over the collection region after the cartridge is positioned in the system. Cover **104** may be a flap coupled to the cartridge that may be moved to uncover or cover the collection region, as desired. Cover **104** may be moved in a sliding motion to cover or uncover the sample collection region. Cover **104** may seal the sample collection region and inhibit contaminants from entering the sample collection region. In some embodiments, the cover may include an opening. Cover **104** may at least partially contain biological waste and/or hazardous materials in the cartridge. In some embodiments, the cover may substantially contain biological waste and/or hazardous materials in the cartridge. In some embodiments, the cover may include an adhesive strip, an absorbent pad, a non-removable plug, a swinging window, a film, a nylon filter or combinations thereof.

[0135] In some embodiments, it may be desirable to inhibit sample from flowing towards a detection region. For example, after a predetermined amount of sample flows towards the detection region, it may be desirable to inhibit more of the sample from flowing towards the detection region. Cover **104** may inhibit undesired additional sample from flowing towards a detection region by absorbing sample from the collection region.

[0136] In some embodiments, a cartridge and/or a body of the cartridge are formed of one or more layers. In certain embodiments, one or more layers seal one or more components in the cartridge. Layers may be coupled, sealed, and/or

bonded together to form the cartridge. The cartridge body may include more than three layers or more than four layers coupled together.

[0137] FIG. 2 depicts an exploded view of an embodiment of a cartridge formed of layers. Cartridge **100** may include top layer **110**, channel layer, **112**, sample layer **114**, reservoir layer **116**, and support layer **118**.

[0138] Top layer **110** may include opening **120**. Samples may be deposited on sample layer **114** through opening **120**. Top layer **110** and support layer **118** may seal cartridge **100**. In some embodiments, each of the layers may include more than one layer coupled together.

[0139] In some embodiments, sample layer **114** may be positioned between one or more channel layers **112** and reservoir layer **116**. Sample layer **114** may include collection region **102** and/or one or more reagent regions **122**. Collection region **102**, one or more fluid channels **106**, and/or reagent regions **122** may be at least partially contained in more than one layer of a body of cartridge **100**.

[0140] Reservoir layer **116** may be positioned proximate sample layer **114**. Reservoir layer **116** may collect sample and/or one or more fluids passing through the cartridge during use. Reservoir layer **116** may include one or more reservoirs **124**, **124'** that collect sample and/or fluid passing through the cartridge (e.g., an overflow reservoir and/or a waste reservoir). In some embodiments, reservoirs may extend through more than one layer. For example, reservoir **124** may extend through channel layer **112** and sample layer **114**.

[0141] Channel layer **112** may be positioned above sample layer **114**. In some embodiments, an additional channel layer may be positioned below a reservoir layer. In certain embodiments, one or more channel layers may be positioned above or below one or more sample layers and/or one or more reservoir layers. Channel layer **112** may include a plurality of channels coupling various components of cartridge **100**. One or more channels **106** may allow fluid to flow within a layer and/or from one layer to another layer.

[0142] In some embodiments, channels are positioned in more than one layer of a cartridge. Positioning a channel in more than one layer may change an elevation of the channel enough to enhance sample and/or fluid to flow in and/or through the cartridge. Channels may be coupled to two or more locations in or on a cartridge. In some embodiments, one or more channels are a part of one or more fluid delivery systems.

[0143] In some embodiments, one or more channels couple a collection region to a detection region, one or more detection systems, and/or one or more overflow reservoirs. Channels may couple one or more fluid delivery systems to a collection region, a detection region, one or more detection systems, and/or one or more reservoirs (e.g., overflow reservoirs and/or one or more waste reservoirs). Two or more channels may be coupled such that they intersect and fluid may optionally flow through more than one channel; however, the size, the elevation, and/or the inside material of the intersecting channel may affect which channel a fluid may flow through and/or may selectively direct fluid flow. Channels or a portion of a channel may promote and/or inhibit fluid flow in or on the cartridge.

[0144] The size and/or the elevation of a channel may selectively direct fluid flow through the channel. Fluid may flow preferentially through a channel that is wider before flowing through narrower channels, thus the fluid may be inhibited from flowing in channels narrower than other proximate

channels. In some embodiments, a portion of the fluid may flow into a narrower channel, while another portion of the fluid flows into a channel wider than the narrow channel. In some embodiments, some channels may have a cross-sectional area larger than a cross-sectional area of other channels of a cartridge. Fluid may flow through the channel with the largest cross-sectional areas prior to flowing through channels with smaller cross-sectional areas. Fluid may be inhibited from flowing into a channel, when the channel has a smaller cross-sectional area than proximate channels.

[0145] In some embodiments, channels include changes in elevation. A portion of a channel may be positioned in a first layer of a cartridge while another portion may be positioned in a second and/or third layer of a cartridge. A channel may have an elevation gradient along an axis parallel to fluid flow. Changes in elevation of a channel may promote, facilitate, and/or increase fluid flow in or on a channel. Elevation changes may inhibit fluid from flowing into a channel.

[0146] In some embodiments channel properties may affect fluid flow in the channels. At least a portion of a channel may selectively direct fluid flow in one or more channels. A channel may be formed of a material, coated with a material or have material deposited on a surface of a portion of the channel that selectively directs fluid flow in one or more channels. For example, a channel may be at least partially formed of a hydrophilic material to promote aqueous fluid flow in the channel. A channel may be at least partially formed of a hydrophobic material to inhibit aqueous fluid flow in the channel. In some embodiments, portions of a channel may be coated with a hydrophilic and/or hydrophobic material. A material that defines at least a part of the channel may be hydrophilic. A channel coupled to a collection region may be partially made of a hydrophilic material to allow an aqueous sample to be drawn from the collection region. In some embodiments, channels partially made of a hydrophobic material may inhibit aqueous fluid flow, thus a waste region may not be needed.

[0147] Channels may be formed of or coated with a hydrophilic material and/or the elevation of the channel may promote fluid flow towards the detection region. In some embodiments, a channel releasing fluid into the detection regions and/or a detection system is at least partially formed of a hydrophilic material to promote laminar flow in the channel. Laminar flow of fluid in the channel may cause matter (e.g., particles, cells, or other matter) in the sample to be evenly distributed across a surface of a portion of a detection system (e.g., a membrane of a membrane-based detection system).

[0148] FIG. 3 depicts an embodiment of a cartridge that includes channels having different elevations. Cartridge 100 may include channels 106, 125, 126, 126', 128, 130, collection region 102, reagent regions 122, 122', detection region 108, overflow reservoir 132, waste reservoir 134, and connectors 136.

[0149] Sample deposited in collection region 102 may flow through channel 106 toward detection region 108. Channel 106 includes metered volume portion 138. Metered volume portion 138 may be a part of the channel. In some embodiments, the metered volume portion is coupled to the channel and/or the collection region. Metered volume portion 138 may have a diameter greater than diameters of proximate channels. If metered volume portion 138 reaches a predetermined amount of fluid (e.g. sample), fluid may flow towards overflow reservoir 132 through channel 125. In some embodi-

ments, substantially all of an introduced sample flows out of collection region 102, into metered volume portion 138. Excess introduced sample will enter overflow reservoir 132 if the metered volume portion is filled. In some embodiments, overflow region 132 is coupled a waste region. Overflow reservoir 132 includes vent 140 to promote fluid flow.

[0150] Vents 140 may be positioned proximate one or more collection regions, metered volume portions, waste reservoirs, overflow reservoirs, and/or in channels coupled to fluid delivery systems. Vents 140 may allow gas to escape from cartridge 100 as fluids pass through or on one or more channels or layers of the cartridge. Vents 140 may inhibit pressure in the channels of the cartridge from becoming greater than ambient pressure. Vents 140 may promote fluid flow in cartridge 100 by releasing pressure associated with the passage of pressurized fluids through the channels. Vents 140 may facilitate laminar flow of fluids in cartridge 100. In some embodiments, vents 140 are designed to inhibit release of fluids through the vent. It may be desirable to limit release of liquids while allowing gas to escape from the cartridge to contain fluids (hazardous reagents and/or biological samples) in the cartridge.

[0151] Channel 106 has different elevations. Different elevations in the channel may inhibit fluid from flowing into detection region 108. It may be desirable to require a sample to be pushed towards a detection system rather than allowing a sample to flow towards a detection system without applied pressure for many reasons. For example, it may be desirable to allow the sample to mix and interact with reagents prior to entering the detection region. Channel 106 may promote fluid flow towards the overflow region. In certain embodiments, channel 106 may have a negative pressure so that fluids are drawn into the channel. In some embodiments, a channel coupled to a collection region may have a negative pressure to draw the sample into the channel.

[0152] Fluid may be delivered to cartridge 100 from one or more fluid delivery systems connected to the cartridge by connectors 136. Connectors may include, but are not limited to, tubing, quick-disconnect connections, and/or locking connectors. It should be understood that any of the various embodiments of fluid delivery systems described herein and/or other fluid delivery systems known in the art may be incorporated with or coupled to cartridge 100.

[0153] Fluid enters channel 126, 126' and passes through and/or over reagent regions 122, 122'. In some embodiments, the reagent region may be a pad, a channel, a depression and/or a reservoir. In some embodiments, the reagent regions may be a part of the fluid delivery system. In some embodiments, the reagent regions are channels, which are a part of a fluid delivery system. Reagent regions 122, 122' may include dried reagents, anti-coagulants, and/or visualization agents. In some embodiments, reagents, buffers and/or visualization agents are dried on or in a pad positioned in or on reagent regions 122, 122'. In some embodiments, reagents and/or visualization agents on and/or in the reagent regions 122, 122' may be reconstituted by fluid passing over and/or the through reagent region.

[0154] Channels 128, 130 may allow fluid to flow from the bottom surface of reagent regions 122, 122' to other components of cartridge 100. In some embodiments, inlet and outlet channels to the reagent regions may be positioned such that fluid is forced to pass through, on, and/or over reagent regions 122, 122'. In some embodiments, additional fluid delivery systems are positioned proximate the reagent regions.

[0155] The fluid delivery system may be controlled to allow fluid to pass across the reagent region 122, enter metered volume portion 138, and then enter detection region 108. Reagents and/or visualization agents in reagent region 122 may be reconstituted by the fluid from the fluid delivery system and may react with the sample. The fluid delivery system may be controlled to allow a predetermined volume of fluid to pass through detection region 108. In some embodiments, fluid from a fluid delivery system may pass over a detection system of the cartridge while the sample incubates on the detection system and/or a membrane of the detection system.

[0156] Channels 128, 130 intersect channel 106, and fluid and/or sample from these channels enters detection region 108 via channel 106. Detection region 108 may include viewing window 142. Viewing window 142 may be optically coupled to a detection system. Viewing window 142 may be positioned in or on the cartridge. Viewing window 142 may be a portion of a detection system. For example, viewing window 142 may be a portion of a top member of a membrane-based detection system located in the detection region. Viewing window 142 may be made of a material transparent to visible or ultraviolet light. Viewing window 142 may include or be composed of a material that acts as a filter that only allows certain wavelengths of light to pass. Viewing window 142 may include a lens that assists in focusing light onto a portion of a detection system and/or onto one or more detectors. A detector may capture an image or light from a detection system through viewing window 142.

[0157] Detection region 108 and/or a detection system in the detection region may be coupled to waste reservoir 134 to allow fluids flowing through the detection system to pass into the waste region. Waste reservoir 134 may be, but is not limited to, a container, a depression, or an opening. Waste reservoir 134 may be coupled to, positioned in, or positioned on the cartridge. By allowing fluids to flow towards a waste reservoir after use, all fluids in the cartridge may be contained within the cartridge. A contained waste reservoir may minimize health and safety hazards due to handling of and/or exposure to the sample and/or fluid.

[0158] Waste reservoir 134 may include cap 144. Cap 144 allows a user to remove fluids from the waste region and/or release pressure from the waste region. All or a portion of cap 144 may be removable. Cap 144 may have a variety of shapes and/or configurations (e.g., round, oval, threaded and/or tapered). A cap on a waste reservoir may allow the waste reservoir to be pressurized so that fluids may be drawn towards the detection system and/or waste reservoir. A waste reservoir may include vent 140 that may inhibit a build up of pressure in the waste reservoir.

[0159] In some embodiments, a fluid delivery system facilitates transport of fluid or sample from one location to another location in or on the cartridge (e.g., from a first location in or on the cartridge to a second and/or third location in or on the cartridge). In certain embodiments, a fluid delivery system delivers reagents, buffer, and/or visualization agents to the detection system. The fluid delivery system may facilitate transport of at least a portion of the sample from the sample collection region to the detection system. The fluid delivery system may couple and/or include channels that couple different regions of the cartridge. For example, the fluid delivery system couples the collection region to the detection system. The fluid delivery system may couple the collection region to the detection system and/or to one or more waste reservoirs.

In some embodiments, the fluid delivery system includes channels that couple components of the analyte-detection system to each other.

[0160] FIG. 4 depicts an embodiment of cartridge 100 with two fluid delivery systems. Cartridge 100 may include channels 106, 125, 126, 126', 128, 130, collection region 102, reagent regions 122, 122', detection region 108, overflow reservoir 132, waste reservoir 134, fluid delivery systems 150, and vents 140. Fluid delivery systems 150 include fluid packages 152, 152' and reservoirs 154. During use, sample may be released from collection region 102, flow through channel 106 and enter detection region 108. Channel 106 may include metered volume portion 138.

[0161] Fluid packages 152, 152' may be opened at predetermined times (e.g., simultaneously or one at a time) to allow fluid (e.g., a buffer, reagent solution or visualization agents) in the fluid package to be released into channel 126, 126'. The released fluids may pass over reagent regions 122, 122' before a portion of sample in channel 106 reaches detection system 108. For example, a portion of a sample is placed in collection region 102 and released into channel 106 after fluid from one of fluid packages 152 flows over and/or through reagent region 122. Alternatively, a portion of sample is placed in collection region 102 and released into channel 106 before and/or simultaneously as fluid from one of fluid packages 152' flows over and/or through reagent region 122'. In some embodiments, substantially the entire excess introduced sample flows out of collection region 102 and into overflow reservoir 132 via channel 125. A size of overflow reservoir 132 may allow fluid from more than one assay to be collected during use.

[0162] Fluid from reagent region 122 flows through channel 128, enters into channel 106, and then enters detection region 108. In some embodiments, channel 128 and channel 106 are the same channel. Channel 126' delivers and/or directs fluid flow from fluid delivery system 150, across and/or through the reagent region 122', and into channel 130. Channel 130, which intersects channel 106, directs fluid from reagent region 122' to a position in channel 106 such that the reagents from reagent region 122' mix with a portion of the sample and/or fluid in channel 106 prior to entering detection region 108. In some embodiments, channel 130 is a part of channel 106.

[0163] Vents 140 may be positioned in or on cartridge 100. Vents 140 may be a part of waste reservoir 134 or a part of one or more channels (e.g., channel 106).

[0164] In some embodiments, valves are used to control fluid flow through the cartridge. Valves may be positioned on or in the cartridge. Valves may direct, control, and/or restrict fluid flow. Active or passive valves may be positioned in channels. Valves may include, but are not limited to, pinch valves, pressure valves, electromagnetic valves, and/or temperature valves.

[0165] In some embodiments, a temperature-controlled valve may be used. A temperature-controlled valve may include a fluid, such as but not limited to, water that is at least partially frozen in a channel to prevent further fluid from passing through the channel. To open the valve, heat is applied to the frozen fluid to melt the fluid. A temperature-controlled valve includes, in some embodiments, a material that is a solid at room temperature (e.g., paraffin or wax). To open a channel, heat may be applied to the solid in the channel to melt the solid material.

[0166] In certain embodiments, a valve is hydraulically activated. In some embodiments, pressurized fluid (e.g., air or water) is used to open or close a valve. Pressure may be transferred via a gas or liquid in a channel to another location in the cartridge. The gas or liquid may be used to compress a drum and/or close a valve. In some embodiments, valves surrounding a portion of a channel having negative pressure inhibit equalizing the negative pressure until desired.

[0167] FIG. 5 depicts cartridge 100 depicted in FIG. 4 with valves 156. Valves 156 are positioned after collection region 102 and after metered volume portion 138. Valves 156 may be used to direct fluid flow from collection region 102 to detection region 108. Valves 156 may be positioned at various other locations in or on cartridge 100.

[0168] FIG. 6 depicts an embodiment of a pinch valve. Pinch valve 158 may include one or more layers 160, 162, 164 and channel 166. Layers 160, 162, 164 may be positioned over a surface of cartridge 100. In some embodiments, the layers are incorporated into the cartridge. Channel 166 may be an opening in cartridge 100.

[0169] Layer 162 may be coupled to layer 160 and layer 164. Surfaces of layers 160, 164 may be composed of materials including, but not limited to, thermal bond film, pressure sensitive adhesive, or other adhesive materials. Layer 162 may be adhered to layers 160, 164 (e.g., using a heat sealing process). In some embodiments, layer 164 forms a wall of channel 166. Layer 162 may be designed so that pressure applied to a surface of layer 162 causes the layer to deform (e.g., layer 162 flexes). Deformation of at least a portion of layer 162 may at least partially obstruct channel 166 as layer 162 is forced into channel 166 by the applied pressure. Layer 162 may be formed of any material that exhibits flexibility when pressure is applied to the layer (e.g., formed of an elastomer material).

[0170] Valves may be activated manually or automatically. In some embodiments, an analyzer system automatically opens or closes the valves. Actuators may be coupled to the analyte-detection system to open and/or close the valves. In some embodiments, an actuator is positioned above the cartridge to apply pressure to a valve through an opening in the cartridge. In some embodiments, an actuator is positioned below the cartridge to apply pressure to a valve through an opening in the cartridge. In some embodiments, actuators are designed to open fluid delivery systems. In some embodiments, a metered volume of a sample including particulate components (e.g., cellular components) may be defined within a cartridge by actuation of one or more valves (e.g., pinch valves).

[0171] In some embodiments, actuation is used to release liquids or gas from a fluid delivery system. Liquids and/or gas may be pressurized into or in the fluid delivery system. An actuated fluid delivery system may be actuated from a top surface, a bottom surface, and/or a side surface of the cartridge. For example, a cartridge may be loaded in a housing of an analyte-detection system with actuators. Actuators are then automatically, semi-automatically, or manually aligned with actuation points of the cartridge. A cartridge positioning system may facilitate cartridge placement into a position such that actuation points are aligned with actuators. Actuation points may be positioned on top, bottom, and/or side surfaces of a cartridge. For example, when a cartridge is positioned in the housing of an analyte-detection system, actuators may be positioned below the cartridge.

[0172] FIG. 7 depicts a perspective top view of a cartridge 100 with an actuator system. The actuator system may include actuators 168, 168', 169, 169' and structure 170. Structure 170 may be designed to move from one side of a cartridge to another side a cartridge 100, along a surface of the cartridge, to facilitate actuation of various valves and/or fluid delivery systems. Structures 170 may be positioned at various points on cartridge 100. As shown, structures 170 are positioned between collection region 102 and detection region 108. Structures 170 may include openings 172. In some embodiments, opening 172 is a track. Actuators 168, 168', 169, 169' may be positioned at various points on or in structure 170 or opening 172. Actuators 168, 168', 169, 169' may move along opening 172 in structure 170, as needed.

[0173] Actuators 168, 168' are positioned over fluid delivery systems 150, 150'. Actuation of fluid delivery system 150 by actuators 168 may force fluid to flow towards metered volume portion 138. Actuation of fluid delivery system 150' by actuator 168' may allow fluid to flow towards reagent region 122.

[0174] Actuators 169, 169' may be positioned over valves proximate metered volume portion 138. Actuation of one or more of the valves proximate meter volume portion 138 may allow a metered volume of sample to flow into and/out of metered volume portion 138. For example, actuator 169 may open the valve between collection region 102 and metered volume portion 138 to allow a portion of a sample to flow into the metered volume portion. Actuator 169' may at least partially open the valve between metered volume portion 138 and detection region 108 to allow a portion of the sample to flow towards the detection region.

[0175] Structure 170 may then be moved to a different location, as desired. In some embodiments, sample in a channel may be inhibited from flowing back towards a collection region by actuating a valve. In some embodiments, one or more actuators may be moved along an opening or a track of the structure until the actuator aligns with a valve. The actuator may then actuate the valve.

[0176] In some embodiments, fluid delivery systems include one or more fluid packages. A fluid package is a package that contains a fluid used by a fluid delivery system. Fluid packages may include liquids or gas under pressure. Fluid packages contain a fluid until the package is opened. Upon opening of the package, fluid in the fluid package may be at least partially released. A fluid package may contain a fluid until an activation pressure is applied to the fluid package. An activation pressure may be the pressure required to release at least a portion of fluids from the fluid package. An activation pressure may be the pressure required to rupture the package of the fluid package. Upon application of an activation pressure to the fluid package, at least a portion of the fluid contained in the fluid package will be released. In some embodiments, a fluid package is activated (e.g., opened) by heat or an electromagnetic signal.

[0177] In some embodiments, fluid packages contain liquids, such as one or more buffers (e.g., phosphate buffers), one or more solvents (e.g., water, methanol, ethanol, and/or THF), one or more reagents, and/or one or more visualization agents. Positioning one or more liquids required for analysis in or on a cartridge may make the fluids more accessible during use and enhance usage of the cartridge. Pre-packaged liquids may limit exposure to the liquids resulting from selection and/or mixing of solutions during use. Pre-packaged liquids may enhance time of analysis from sample collection

to analysis of the sample. Placing the liquids required for analysis in fluid packages may increase stability and/or shelf life of a cartridge that includes an actuated fluid delivery system. Additionally, fluid packages may allow the cartridge to be stored at room temperature rather than requiring refrigeration.

[0178] In some embodiments, a fluid package includes a solvent. The solvent in a fluid package may be released from the fluid package and flow over one or more reagent pads that include buffer chemicals, reagents, and/or visualization agents. A cartridge including solvent filled fluid packages and dried buffers, reagents, and/or visualization agents may increase the stability of the cartridge since dried buffers, reagents, and visualization agents may be more stable and/or may have a greater shelf life than aqueous solutions.

[0179] In some embodiments, a fluid package delivers air or another gas to the cartridge. Gas released from a fluid package may assist in transporting a fluid and/or a sample through and/or in the components and/or channels of the cartridge.

[0180] In certain embodiments, a fluid package is designed to be filled with fluid with substantially few or no air bubbles. A fluid package may be designed to inhibit release of air bubbles or gas within a fluid package into a cartridge channel or component during partial or full compression and/or actuation of the fluid delivery system.

[0181] In some embodiments, a fluid package is designed to release at least 80 percent of liquid or gas contained in the fluid package. A fluid package may include about 1 mL to about 500 mL of fluid. In certain embodiments, a fluid package has a shelf life of at least 2 years and/or has a volume loss of less than 5 percent of the original volume during a 2-year period.

[0182] A fluid package may be, but is not limited to, a pouch, container, and/or chamber. The fluid package may be formed from plastic materials. Plastic material may allow the fluid package to deform and release fluid. Once the fluid is released the plastic fluid package does not attempt to reform, thus creation of at least a partial vacuum is inhibited. Creation of at least a partial vacuum may draw fluids and/or gas back into the fluid package.

[0183] In some embodiments, a fluid package may be deformable in a controlled manner. The fluid package may be formed of a material that allows the fluid package to be deformed and/or compressed (e.g., elastomeric material). A deformable/compressible material may allow a fluid package to be transported, stored, and/or positioned without breakage.

[0184] A fluid package may be made of materials including, but not limited to, polyvinyl chloride (PVC), polyvinylidene chloride (PVDC), polyethylene (PE), rubber, polypropylene (PP), polyacrylonitrile (PAN), cyclic olefin copolymer (COC), fluoropolymer films, foil (e.g., aluminum foil or plastic foil), adhesive tapes, or combinations thereof.

[0185] In some embodiments, a fluid package may be formed of a first material and a second material, where a second material is designed to rupture or break before the first material when pressure is applied to the fluid package. In some embodiments, a wall of the fluid package may be formed of layers of polypropylene and cyclic olefin copolymer.

[0186] A fluid package may be formed of a material compatible with the fluid it is designed to contain. A fluid package may be formed of a material that will not leach into the fluid contained within the fluid package. In certain embodiments, a

fluid package includes a layer that couples the fluid package to the cartridge. The layer may be formed of a material capable of bonding (e.g., adhesive material) to acrylic, plastics, and/or other materials used to form a cartridge body.

[0187] A wall of a fluid package may be designed to have a weak portion (e.g., a burst point). The weak wall portion may rupture when a predetermined amount of pressure is applied to the fluid package. Fluid may be released from a fluid package when by applying sufficient pressure to the package to cause the weak wall portion to rupture. The location of the weakened wall portion may be aligned with or coupled to a channel and/or component opening. A fluid package may be designed with a burst point or point at which fluid is released of about 3 psi to about 7 psi.

[0188] FIG. 8 depicts a side view of an embodiment of a fluid package. FIG. 9 depicts a top view of the embodiment of the fluid package depicted in FIG. 8. Fluid package 152 may be coupled to, at least partially positioned in, or at least partially positioned on cartridge 100. As depicted in FIG. 9, fluid package 152 may include layer 174. Layer 174 may be made of material (e.g., adhesive) that allows fluid package 152 to couple to cartridge 100. Fluid package 152 may be at least partially filled with liquid. Fluid package 152 may include liquid 176 and gas 178. Examples of gas 178 are air, nitrogen, and/or argon. A portion of a wall of fluid package 152 may include a burst point. As pressure is applied to the fluid package 152, wall 180 of fluid package 152 may rupture at the burst point. Once fluid package 152 ruptures, fluid may be released from the fluid package into channel 106. The rigidity of fluid package 152 may be modified to accommodate various applications and/or storage or transport conditions. In some embodiments, fluid and/or air may be contained in the fluid package by a removable adhesive strip. Removal of the adhesive strip may allow fluid and/or air from the fluid package to be released from the fluid package.

[0189] In some embodiments, a cartridge includes a projection to rupture a portion of the fluid package. The projection may be needle shaped or any other shape capable of perforating a fluid package. The projection may be formed from any suitable material such as metal, plastic, and/or silicon. FIG. 10 depicts a side view of an embodiment of a fluid package positioned in a cartridge with a projection. Projection 182 may be positioned proximate to a surface of fluid package 152 and/or cartridge 100. Cover 184 may be positioned over fluid package 152. FIG. 11 depicts an embodiment of rupturing the fluid package depicted in FIG. 10. When pressure is applied to cover 184, the cover contacts the fluid package 152 causing the fluid package to contact projection 182. Projection 182 may rupture a portion of fluid package 152 causing fluids to be released channel 106.

[0190] FIG. 12 depicts cross-sectional view of a fluid package positioned in cartridge 100. Fluid package is positioned in opening 154 of cartridge 100. In some embodiments, fluid package is positioned on the cartridge. In some embodiments, one or more walls of the opening are capable of being deformed (e.g., the walls flex). Cover 184 may be positioned above opening 154. Cover 184 may be formed of an adhesive so that fluid package 152 is retained in opening 154. Projection 182 may be coupled to cartridge 100. Pressure applied to cover 184 may cause wall 180 of fluid package 152 to contact projection 182 and rupture. Fluid from fluid package 152 may be released into channel 106. Baffles 200 positioned proximate the bottom of opening 154 may assist in controlling flow rate of the fluid from fluid package 152.

[0191] In some embodiments, a fluid delivery system includes one or more fluid packages and a reservoir. The one or more fluid packages may be sealed and/or positioned in the reservoir. The reservoir may be coupled to, positioned in or positioned on the cartridge.

[0192] FIG. 13 is a perspective view of a fluid delivery system with a fluid package and a reservoir. Fluid delivery system 150 may include fluid package 152, reservoir 154, and support 188. In some embodiments, support 188 is part of a cartridge body. Portions of the fluid delivery system may be formed of several layers. In some embodiments, portions of the fluid delivery system may be formed of silicon resin, double-sided adhesive, thermo-bond film, and/or metal foil.

[0193] FIG. 14 depicts an exploded view of fluid delivery system 150 depicted in FIG. 13. Support 188 may include support layer 189, channel layer 190, middle layer 192, and top layer 194. Support layer 189 and/or middle layer 192 may assist in retaining fluids in channel layer 190. Support layer 189 may be a portion of a cartridge. Support layer may be formed of plastic and/or glass. Channel layer 190 may be coupled to, or be a part of, support layer 189. Channel 106 of channel layer 190 directs fluid flow to a collection region and/or a detection region of the cartridge. Channel layer 190 may include reagent regions and/or have properties described herein. In some embodiments, the layers of fluid delivery system 150 may be the same as the layers in cartridge 100.

[0194] Middle layer 192 may be coupled to or be a part of channel layer 190. Portions of middle layer 192 may include coupling agents (e.g., adhesive or adhesive film) that couple the middle layer to channel layer 190. Middle layer 192 may include opening 196. Opening 196 may direct fluid into channel 106. Middle layer 192 may be coupled to top layer 194 using generally known coupling techniques (e.g., adhesive, pins, and/or screws).

[0195] Top layer 194 may seal or contain fluids in fluid package 152 and/or reservoir 154. Top layer 194 may include opening 198. Opening 198 may direct fluid from fluid package 152 and/or reservoir 154 to channel layer 190. Top layer 194 may include seal 202. Seal 202 may be positioned between middle layer 192 and top layer 194. Seal 202 may cover opening 198 of top layer 194. Seal 202 may seal fluid and/or gas in fluid package 152 and/or reservoir 154. Seal 202 may be formed from a variety of materials (e.g., thermo-bond film, and/or foil). Seal 202 may rupture when pressure is applied to fluid package 152 and/or reservoir 154. In some embodiments, seal 202 may be a part of top layer 194.

[0196] Top layer 194 may be coupled to or be a part of reservoir 154 using generally known coupling techniques. Reservoir 154 may include opening 203. Reservoir opening 203 may be aligned with top layer opening 198. Top layer 194 may be coupled to or be a part of reservoir 154 and/or fluid package wall 180.

[0197] Fluid package 152 may be positioned in reservoir 154. A wall of fluid package 152 may be aligned with reservoir opening 203 and top layer opening 196. A portion of a wall of fluid package 152 includes a burst point to allow the fluid package to rupture when a predetermined amount of pressure is applied to the fluid package and/or reservoir 154. In some embodiment, the fluid package and the reservoir are one unit. In some embodiments the reservoir does not include the fluid package.

[0198] FIG. 15 depicts a perspective cut-away view of the reservoir of fluid delivery system 150 depicted in FIG. 13. A diameter of top layer opening 198 and/or the reservoir open-

ing may be less than, equal to, or greater than a diameter of than middle layer opening 196. As depicted, seal 202 has been torn to allow fluid to flow to channel 106 in channel layer 190. A center of seal 202 may be directly aligned or offset with a center of top layer opening 198.

[0199] FIG. 16 depicts a cut-away perspective view of top layer 194 and reservoir 154 containing fluid package 152 as depicted in FIG. 13. FIG. 17 depicts a top view of fluid reservoir 154. As seen in FIG. 17, seal 202 is offset from top layer opening 198 in top layer 194. Offsetting seal 202 may facilitate the rupturing of the seal when a predetermined amount of pressure is applied to the fluid package and/or reservoir by creating a weak point in the seal.

[0200] A center of the seal may be offset from the center of the top layer opening by a distance ranging from about 0.2 mm to about 2 mm, about 0.3 mm to about 1.5 mm, or about 0.4 mm to about 1 mm. When the center of the seal is offset from the center of the top cover opening by about 0.25 mm, a burst point of the seal may rupture at a pressure of about 1 psi to at most 10 psi, from about 3 psi to about 8 psi, or from about 5 psi to about 7 psi. In contrast, the burst point of the seal may rupture at a pressure of greater than 10 psi when a center of the seal is aligned with the center of the top cover opening.

[0201] In some embodiments, the pressure required to rupture a fluid package is lowered by varying the materials used to create the seal, decreasing the surface area of the seal in a strategic location, decreasing the bonding temperature of the seal, and/or decreasing the time of heat sealing the seal to the top layer and/or the reservoir. Application of force to the reservoir and/or the fluid package may change the internal pressure in the reservoir and/or the fluid package enough to cause the seal to rupture or separate from the top layer. Rupturing or separating the seal from the top layer allows fluids in the reservoir to pass through the reservoir opening, the top layer opening, and/or the cover layer opening and into the channel layer.

[0202] In some embodiments, a fluid package is coupled to a structure (e.g., a planar support or a cartridge). The structure may provide support for the fluid package. FIG. 18 depicts an embodiment of fluid delivery system 150 that includes fluid package 152 coupled to support 188 (e.g., a cartridge). FIG. 19 depicts an exploded view of fluid delivery system 150 depicted in FIG. 18. Support 188 may include support layer 189, channel layer 190 and top layer 194. Channel layer 190 may be coupled to support layer 189 and top layer 110. Channel layer 190 may be at least partially formed from double-sided adhesive. Channel layer may include channel 106.

[0203] Top layer 194 and support layer 189 may seal fluids in channel layer 190. Top layer 194 may include opening 198. Top layer opening 198 may direct fluid from fluid package 152 to channel layer 190. Top layer 194 or a portion of the top layer may include a material capable of coupling the top layer to fluid package 152 (e.g., vinyl adhesive or other types of adhesive). In some embodiments top layer 194 and fluid package 152 are formed as one unit.

[0204] FIG. 20 depicts an embodiment of the fluid package depicted in FIG. 18 and FIG. 19. Fluid package 152 may include walls 204. Walls 204 may be formed of a material that allows the walls to be rigid while being able to collapse. Walls 204 may be corrugated and designed to fold. For example, walls 204 may form a shape similar to an accordion. Walls 204 may have limited outward flexibility under pressure. A corrugated fold may maximize the efficiency of the fluid

package to deliver fluid. Walls **204** may be designed such that compression (full or partial) of the fluid package will not cause the base of the fluid package to flex upwards and/or cause the walls of the fluid package to flex outwards. In some embodiments, a diameter of the fluid package base is larger than a diameter of the fluid package opening and the top layer opening. The larger base may enhance bonding of the fluid package to the top layer. In some embodiments, fluid package **152** may have a rigid and/or ridged top surface. The rigid and/or ridged top surface may allow an actuator to contact the fluid package without puncturing the fluid package. The actuator may apply pressure to the top surface to force fluid from the fluid package.

[0205] FIG. 21 depicts an exploded view of a fluid delivery system that may be coupled to a support. Fluid delivery system **150** may include reservoir **154**, gasket **206**, and seal **202**. Reservoir **154** includes one closed end and one open end. In some embodiments, the reservoir is formed from a mold made from Delrin (DuPont, Wilmington, Del.), an inflexible polymer, brass, stainless steel, and/or aluminum. For example, reservoir **154** may be molded from polydimethylsiloxane. The open end of reservoir **154** may include flange **205**. Gasket **206** may couple flange **205** to seal **202**. Seal **202** may be coupled to an opening in a top layer. Gasket **206** may include burst point **208**. When a predetermined pressure is applied to reservoir **154**, gasket **206** may rupture at burst point **208** causing seal **202** to rupture and/or tear. Rupturing of seal **202** allows fluid from reservoir **154** to flow through the opening in the top layer to a channel layer of the cartridge. In some embodiments, gasket **206** is a double-sided adhesive layer.

[0206] In some embodiments, a fluid delivery system includes a flexible conduit with a negative pressure source. The negative pressure source may be a fluid package. The negative pressure source may have a pressure less than ambient pressure. FIG. 22A depicts fluid package **152** as a negative pressure source before actuation. FIG. 22B depicts fluid package **152** as a negative pressure after actuation. When a negative pressure source is actuated (e.g., a seal is removed, a seal is ruptured, or a conduit is inserted in a wall or seal of the negative pressure source), air and/or fluid are drawn towards the negative pressure source until the pressure equalizes (the negative pressure source inflates). Actuating or opening a negative pressure source may create at least a partial vacuum in one or more channels.

[0207] A fluid delivery system may include a fluid bulb coupled, integrated, or embedded into the cartridge. A cartridge may be designed to incorporate commercially available fluid bulbs or custom designed fluid bulbs. Fluid bulbs may have various dimensions depending on dispensing volumes required and/or cartridge specifications.

[0208] FIG. 23 depicts an embodiment of a fluid bulb. Fluid bulb **210** may include body **211**, and conduit **212**. Conduit **212** may be straight, angled and/or tapered. Conduit **212** may include tip **214**. In some embodiments, tip **214** may be a breakaway sealed tip. Tip may be angled **214**. Tip **214** may couple or removably couple to a cartridge.

[0209] FIG. 24 depicts an embodiment of a fluid bulb **210** coupled or removably coupled to a channel in the cartridge. Body **211** may release liquid **176** upon actuation. Body **211** may be coupled, via conduit **212**, to connector **216**. Connector **216** may connect fluid bulb **210** to channel **106** of the cartridge. In some embodiments, tip **214** may be positioned in connector **216**. In certain embodiments, the connector may include one or more openings to allow more than one fluid

delivery system to be attached to the connector. Connector **216** may be permanently affixed to conduit **212**. In some embodiments, connector **216** may be removably coupled to conduit **212** and/or channel **106**.

[0210] In some embodiments, a fluid delivery system may include one or more syringes coupled, embedded, or integrated into the cartridge. Syringes may be used to provide fluid delivery control, volume control, and/or a secure fluid seal to a cartridge. A syringe may be formed from a biocompatible material. Syringes may have a variety of designs, such as but not limited to, the embodiments depicted in FIGS. 25A-25H. The dimensions of syringes **218** may vary depending on dispensing volumes required and/or cartridge specifications. Use of a syringe in a fluid delivery system may offer accurate and/or precise fluid delivery. In some embodiments, pre-filled syringes may be positionable in a cartridge prior to use.

[0211] FIG. 26A depicts an embodiment of a cartridge that includes syringes **217**, **218**, **219**. Syringes **217**, **218**, **219** may be linearly activated simultaneously or sequentially. Syringes **217**, **218**, **219** may be actuated when a prong contacts the fluid delivery system. In some embodiments, an actuator with three prongs of different lengths may be actuated to release fluid from the syringes. Using an actuator with prongs of different lengths may allow actuation of different syringes at different times using a single actuation of the prongs. Since the prongs are of different lengths, the actuation system may be set up such that each prong contacts a syringe at a different, predetermined, time. As each prong of the actuator depresses a syringe, fluid may be released. Syringes **217**, **218**, **219** may deliver fluid to various portions of the cartridge. For example, syringe **217** may deliver a fluid toward reagent region **122**, while syringe **218** delivers fluid towards metered volume portion **138**.

[0212] An expanded view of one the end of syringe **219** is depicted in FIG. 26B. Syringe **219** includes tip **214** positionable in connector **216**. In some embodiments, connector **216** is coupled to the cartridge. Tip **214** may be designed to mate with connector **216**. In some embodiments, a tip may include adhesive and/or a gasket to seal the syringe to the connector. A cartridge may include a spring mechanism that holds the syringes in position.

[0213] In some embodiments, a metered syringe pump is used to push and pull fluids through the system. During use, a capillary containing sample may be inserted into the cartridge coupled to a fluid bus. The system may then be filled with buffer through two lines. Using a third line, sample may be pushed into a trap that releases air trapped in the sample. A line may then be used to draw a predetermined amount of sample into the detection system. After sample analysis, the system may be washed with a buffer solution and waste may be transferred to a waste reservoir positioned in the cartridge or coupled to the cartridge.

[0214] In some embodiments, an analyte-detection system may be used to test for multiple analytes. The analyte-detection system may include a multi-functional cartridge. The multi-functional cartridge may include two or more detection systems. In some embodiments, a single cartridge or system may include a membrane-based detection system and a particle-based detection system. The membrane-based detection system may be positioned upstream from the particle-based detection system. A sample may be introduced into the cartridge or system and passed through the membrane-based detection system where a portion of the sample is retained by

the membrane. The material passing through the membrane may be passed to the particle-based detection system. Particles in the particle-based detection system may interact with one or more analytes in the fluid passed over the particles. In alternate embodiments, a particle-based detection system may be positioned upstream from a membrane-based detection system. In certain embodiments, particles may be coupled to (e.g., at least partially embedded in) at least a portion of a membrane of a membrane-based detection system. In combination, the two detection systems allow the presence of at least two analytes to be assessed in a single sample at about the same time.

[0215] FIG. 27 depicts perspective top view of an embodiment of a cartridge that includes two detection systems. Cartridge 100 may include fluid delivery systems 150, reagent regions 122, collection region 102, membrane-based detection system 220, particle-based detection system 222, and waste reservoir 134.

[0216] Sample may be deposited in and/or delivered to collection region 102. In some embodiments, a filter may be positioned proximate the collection region to allow removal of large particles and/or coagulated matter from the sample. In some embodiments, fluid may be released from fluid delivery systems 150 directly into channel 106. In some embodiments, fluid from the fluid delivery system may flow directly to one of the detection systems (e.g., flow directly to the membrane-based detection system).

[0217] Fluid may be released from fluid delivery systems 150 and pass through reagent region 122. Reagent region 122 may include dried reagents, anti-coagulants, and/or visualization agents. In some embodiments, reagents and/or visualization agents on and/or in the reagent pad may be reconstituted by fluid passing over and/or through reagent region 122. In some embodiments, reagent region 122 includes reagent pads that contain dried reagents, anti-coagulants, and/or visualization agents. A reagent pad acts, in some embodiments, as a filter and removes large particles and/or coagulated matter from the sample.

[0218] In some embodiments, a reagent region may be positioned proximate the collection region so that sample from the collection region may pass over the reagent pad and reconstitute reagents and/or visualization agents in the reagent region. Directly flowing sample over and/or through a reagent region may facilitate the time of reaction between sample and reagents and/or visualization agents.

[0219] After fluid flows through and/or over reagent region 122, fluid may flow over and/or through collection region 102. A combined fluid and sample flows toward the membrane-based detection system 220 and particle-based detection system 222. In some embodiments, a combined fluid and sample passes through the particle-based detection system first. In certain embodiments, a combined fluid and sample may first pass through a first detection system for a first test and only pass through the second detection system based on the results of the first test.

[0220] Membrane-based detection system 220 and/or particle-based detection system 222 may be coupled to waste region 134. Fluid may flow from membrane-based detection system 220 and then to particle-based detection system 222 to waste region 134.

[0221] In some embodiments, a cartridge of an analyte-detection system may be multi-functional (e.g., used to analyze two or more analytes in a sample). In some embodiments, the analysis may be done simultaneously, or

substantially simultaneously. For example, a cartridge may be used to assess WBC count and CRP levels in a whole blood sample.

[0222] FIG. 28 depicts a top view of an embodiment of multi-functional cartridge 100. Cartridge 100 may include connectors 136, 136', channels 106, 126, 128, 130, metered volume portion 138, collection region 102, reagent regions 122, 122', overflow reservoir 132, membrane-based detection system 220, particle-based detection system 222, waste reservoir 134, and vents 140.

[0223] Sample may be deposited in collection region 102. Sample flows from collection region 102 through channel 106 and enters metered volume portion 138. Sample may then be delivered to membrane-based detection system 220 from metered volume portion 138. Excess sample may be collected in overflow reservoir 132.

[0224] Connectors 136, 136' may connect one or more fluid delivery systems to the cartridges. Fluid from the fluid delivery systems flows through channels 126 to reagent regions 122, 122', respectively. Fluid may be delivered at different time intervals or substantially simultaneously to the reagent regions from separate fluid delivery systems. In some embodiments, fluid from the fluid delivery system may flow directly to one of the detection systems (e.g., flow directly to the membrane-based detection system).

[0225] Fluid may pass through or over reagent region 122, through channel 128 and enter metered volume portion 138. Fluid may be delivered to membrane-based detection system 220 from metered volume portion 138. Excess fluid and/or sample may be collected in overflow reservoir 132.

[0226] A similar fluid or different fluid that passed through or over reagent region 122 may pass through or over reagent region 122'. Fluid from reagent region 122' flows toward membrane-based detection system 220 through channel 130. In some embodiments, an additional amount of sample is delivered from metered volume portion 138 to membrane-based detection system 220 before fluid from reagent region 122' reaches the membrane-based detection system. In some embodiments, fluid from reagent region 122' may flow directly to particle-based detection system 222.

[0227] Sample and/or fluid that pass through or over membrane-based detection system 220 is transported to particle-based detection system 222. The detection systems may be optically coupled to a detector and the analytes in the sample may be analyzed. In some embodiments, the analytes in the sample retained in membrane-based detection system 220 may be analyzed prior to sending the remainder of the sample to the particle-based detection system 222. In some embodiments, the sample may be transported to the particle-based detection system 222 before being delivered to the membrane-based detection system 220.

[0228] Membrane-based detection system 220 and/or particle-based detection system 222 may be coupled to waste region 134. Fluid may flow from membrane-based detection system 220, to particle-based detection system 222, and then to waste region 134.

[0229] FIG. 29 depicts an exploded view of the embodiment of cartridge 100 depicted in FIG. 28. Cartridge 100 includes top layer 110, top layer opening 120, sample layer 114, reservoir layer 116, reservoirs 124, support layer 118, and connectors 136 designed to couple to fluid delivery systems. In certain embodiments, one or more additional fluid delivery systems (e.g., fluid packages) may be coupled to,

positioned on or positioned in cartridge **100** to provide fluid for sample processing during use.

[0230] Cartridges described herein may include a membrane-detection system. A membrane-detection system may include a membrane and, optionally, a membrane support. The membrane may retain at least a portion of matter in the sample, while allowing other portions of the sample to pass through the membrane. For example, with blood samples, a membrane may be selected that will allow red blood cells and plasma to pass through the membrane, while the membrane retains white blood cells.

[0231] FIG. **30** depicts an embodiment of a membrane-based detection system. The membrane-based detection system may be coupled to, positioned in, or positioned on cartridge **100**. The membrane-based detection system may be integrated within a cartridge.

[0232] Membrane-based detection system **220** includes membrane **226** and membrane support **228**. In some embodiments, a membrane may be designed such that a membrane support is not necessary. For example, a thickness of a membrane may be selected so that a membrane remains substantially planar. In some embodiments, the membrane is porous.

[0233] The membrane-based detection system **220** may include housing **230** positioned on a cartridge **100**. Bottom spacer **232** may position bottom member **234** in housing **230**. Bottom member **234** may include indentation **236** to receive membrane **226** and membrane support **228**. Channel **238** in bottom member **234** may receive fluids flowing through membrane **226** and conduct the fluids to outlet **240**. In some embodiments, the outlet is coupled to a waste reservoir of the cartridge. Gasket **242** may be positioned between top member **244** and membrane **226**. Gasket **242** may reduce leaks from the membrane-based detection system. Inlet **246** coupled to top member **244** may allow fluids to enter the membrane-based detection system. Top spacer **248** may be positioned between top member **244** and fastening member **250**. Top member **244** may include viewing windows **142**. Viewing windows **142** may be transparent to visible light and/or ultraviolet light. Fastening member **250** may keep the components of the membrane-based detection system coupled during use. Fastening member **250** may be machined (e.g., threaded and/or tapered) to mate with housing **230**.

[0234] In some embodiments, a membrane-based detection system may include layers to direct fluid flow. FIG. **31** depicts an exploded view of an embodiment of a membrane-based detection system with directed fluid flow. The membrane-based detection system may include a plurality of layers positioned in the cartridge or on a surface of the cartridge. Membrane-based detection system **220** includes top member **244**, top layer **252**, middle layer **254**, membrane **226**, bottom layer **256**, and membrane support **228**. Layers of the membrane-based detection system may be coupled to each other. Top layer **252**, middle layer **254**, and bottom layer **256** may include openings **258**, **260**, and **262**, respectively. Fluid may flow from inlet **246** through openings **258** and **260** to and/or through membrane **226**. A portion of analytes in the fluid flowing to the membrane **226** may be retained on the membrane. Light may be directed to a portion of the membrane to detect analytes in the fluid. Fluid may flow through membrane **226**, through opening **262** and out through outlet **240** to one or more reservoirs.

[0235] In some embodiments, a cavity is formed between the top member and the membrane. The top member may be spaced at a distance above the membrane to form the cavity

and/or the top member may have a shape such that a cavity is formed between the top member and the membrane.

[0236] Top member **244** may be at least partially transparent to visible light and/or ultraviolet light. Top member **244** is, in some embodiments, formed of PMMA. Top member **244** may include viewing window **142**. In some embodiments, a portion of top member **244** may be opaque or translucent to visible light and/or ultraviolet light while viewing window **142** may be substantially transparent to visible light and/or ultraviolet light.

[0237] Fluid may be directed towards membrane **226** through top layer **252** positioned below top member **244**. A portion of top layer **252** may be formed of a material or materials (e.g., vinyl material and/or an adhesive) capable of coupling the top layer to middle layer **254**. Top layer **252** may direct flow of fluid from top member **244** through opening **258** and towards membrane **226**.

[0238] Middle layer **254** may be positioned below top layer **252**. Middle layer **254** may be formed of a vinyl material and/or adhesive. A portion of middle layer **254** may be formed of a material or materials (e.g., vinyl material and/or an adhesive) capable of coupling the middle layer to top layer **252** and/or bottom layer **256**. Middle layer **254** may be opaque or translucent to visible light and/or ultraviolet light. Middle layer **254** may direct fluid to flow through opening **260** toward membrane **226**.

[0239] Fluid that flows through membrane **226** passes through opening **262** in bottom layer **256**. Bottom layer **256** may direct fluid flow through opening **262**. A portion of bottom layer **256** may be formed of a material or materials (e.g., vinyl material and/or an adhesive) capable of coupling the bottom layer to middle layer **254**. In some embodiments, opening **262** in bottom layer **256** has a size similar to the size of opening **260**. Openings with similar sizes may allow fluid to be retained in the area of membrane **226** between the middle layer **254** and bottom layer **256**.

[0240] Gasket **242** may be positioned below bottom layer **256** to inhibit leaks from the membrane-based detection device. Membrane support **228** may be positioned below gasket **242**. In some embodiments, membrane support **228** may inhibit sagging of membrane **226**. Membrane support **228** may be positioned in bottom member **234** and/or an opening of the cartridge. Bottom member **234** may include indentation **236** to receive membrane **226** and/or membrane support **228**. Channel **238** in bottom member **234** may receive fluids flowing through membrane **226** and conduct the fluids to outlet **240**.

[0241] In some embodiments, a membrane is selected depending on the analyte of interest. The membrane may capture or retain matter in the sample (e.g., particles, cells, or other matter). Matter may be retained on a surface of the membrane and/or in the membrane. The membrane may include a thin film or layer capable of separating one or more components from a liquid passing through the film or layer. The surface of a membrane may be hydrophilic to promote cell proliferation across the surface of the membrane. A membrane may have a variety of shapes including, but not limited to, square, rectangular, circular, oval, and/or irregularly shaped. In some embodiments, a membrane includes openings (e.g., pores) that inhibit an analyte of interest from passing through the membrane. A membrane designed to capture substantially all of an analyte of interest may be selected depending on the analyte of interest.

[0242] In some embodiments, a membrane is a monolithic microchip with a plurality of high-density holes. The monolithic microchip membrane may be formed from materials including, but not limited to, glass, silica/germanium oxide doped silica, inorganic polymers, organic polymers, titanium, silicon, silicon nitride, and/or mixtures thereof. Organic polymers include, but are not limited to, PMMA, polycarbonate (PC) (e.g., NUCLEOPORE® membranes, Whatman, Florham Park, N.J.), and resins (e.g., Deirin®). A membrane formed of polymeric material may include pores of a selected range of dimensions. In certain embodiments, a membrane is an acrylic frit. In some embodiments, a membrane is formed of multiple layers (e.g., at least 2 layers, at least 3 layers, at least 4 layers, or at least 5 layers) of etchable and/or nonetchable glass. In some embodiments, a membrane is formed from an anti-reflective material and/or a material that does not reflect light in the ultraviolet-visible light range. In some embodiments, a membrane includes one or more locking mechanisms to assist in securing placement of the membrane in or on the cartridge or membrane support.

[0243] In some embodiments, membranes are microsieves. Microsieves may be manufactured from silicon materials and/or plastic materials. In some embodiments, a microsieve is a layered plastic microsieve.

[0244] Membranes may have a thickness from about 0.001 mm to about 25 mm, from about 1 mm to about 20 mm, or from about 5 mm to 10 mm. In some embodiments, a thickness of the membrane ranges from about 0.001 mm to about 2 mm. Membranes may have a diameter from about 1 mm to 500 mm, from about 5 mm to about 100 mm, or from about 10 mm to about 50 mm.

[0245] Pores of a membrane may have various dimensions (e.g., diameter and/or volume). In some embodiments, pores of the membrane may have approximately the same dimensions. In some embodiments, membrane pores have a pore diameter ranging from about 0.0001 mm to about 1 mm; from about 0.0002 mm to about 0.5 mm; from about 0.002 mm to about 0.1 mm. The membrane pores have, in some embodiments, a pore diameter of at most 0.005 mm or at most 0.01 mm.

[0246] Pores of the membrane may be randomly arranged or arranged in a pattern (e.g., a hexagonal close-packed arrangement). Pores of the membrane may occupy at least 10 percent, at least 30 percent, at least 50 percent, or at least 90 percent of the surface area of a membrane. The pores may assist in selectively retaining matter in a sample and/or a fluid.

[0247] In some embodiments, a membrane is positioned from about 0.3 mm to about 0.5 mm below a top surface of the cartridge. In some embodiments, the membrane includes a support. In some embodiments, a membrane is designed such that a membrane support is not needed (e.g., utilizing a membrane having a thickness of at least 5 mm). In some embodiments, one or more layers separate the membrane and the membrane support. The membrane support may facilitate positioning of the membrane in or on the cartridge.

[0248] A membrane support may be coupled to the cartridge or integrated within a cartridge. In some embodiments, a membrane support is used to maintain a membrane in a substantially planar orientation. In certain embodiments, a membrane support is integrated with one or more membranes. The membrane support may be formed of the same material as the membrane. The membrane support may be formed of materials including, but not limited to, glass, polymers, metal, silicon, PC, cyclic olefin copolymer (COC),

nylon, and/or nitrocellulose. The membrane support may be, but is not limited to, a stainless steel filter or a plastic mesh.

[0249] A support assembly may be coupled to the membrane support to allow the membrane and membrane support to withstand backpressures of at least 10 psi. The membrane support may be selected to produce a predetermined backpressure. When backpressure is controlled, cells may be more uniformly distributed across a surface of a membrane. Uniform distribution of cells across a membrane surface may facilitate imaging of a region containing cells and/or analyte detection.

[0250] In some embodiments, a membrane support includes open areas (e.g., pores or holes). Open areas in the membrane support may have any shape, such as substantially square and/or substantially circular. The shape of the open areas in the membrane support may be different than the shape of pores in the membrane. Open areas of the membrane support may be equal to or greater than the diameter of the pores of the membrane. In some embodiments, a membrane support has open areas with diameters ranging from about 0.0001 mm to about 1 mm, from about 0.0002 mm to about 0.5 mm, or from about 0.002 mm to about 0.1 mm. The open areas have, in some embodiments, diameters of at most 0.005 mm or at most 0.01 mm.

[0251] FIG. 32 depicts a top view of an embodiment of a membrane support having a parallelogram shape. Membrane support 228 may include outer area 264 and open area 266. Open area 266 may include openings 268. Membrane support 228 may be machined and/or fabricated such that open area 266 has various shapes. Various shapes of open area 266 may allow particles of different sizes to be removed during analysis of the analyte. Length (L) of outer area 264 may be greater than or about equal to width (W) of the outer area (e.g., outer area 264 may have a substantially square shape or a substantially rectangular shape). A length of open area 266 may be greater than, or about equal to a width of the open area (e.g., open area 266 may have a substantially square shape or a substantially rectangular shape). Open area 266 may have dimensions that are less than the dimensions of outer area 264. In some embodiments, an outer area of a membrane support may have a length about 4 mm to about 6 mm and a width from about 4 mm to about 6 mm. An open area of a membrane support may have a length from about 2.5 mm to about 4 mm and a width from about 2.5 mm to about 4 mm. FIG. 33 depicts a top view of an embodiment of membrane support 228 having an euclidian shape (e.g. membrane support 228 have a substantially oval shape or a substantially circular shape). Open area 266 may have dimensions that are less than the dimensions of outer area 264.

[0252] FIG. 34 depicts a perspective cross-sectional view of open area 266 of membrane support 228. Open area 266 includes top portion 270 and bottom portion 272. Bottom portion 272 may be equal to or less than the top portion 270. In some embodiments, a membrane support may include a top portion formed from a silicon nitride film and a bottom portion formed from silicon. A membrane support may be formed from a hydrophilic and/or anti-reflective material. Forming a membrane support from a hydrophilic material may reduce the formation of air bubbles across the membrane and membrane support. Use of a hydrophilic material may also inhibit nonspecific binding of analytes. Using a membrane support made at least partially of anti-reflective material may enhance analyte detection.

[0253] In embodiments where the membrane support is formed from silicon, a bottom portion of the membrane support has a thickness (T) ranging from about 0.001 mm to about 5 mm. For silicon membrane supports, a thickness of the membrane support is related to a length (Lt) of the top portion 270 and a length (Lb) of the bottom portion 272 as represented by the equation:

$$T = \tan(54.7^\circ) \times (L_t - L_b) / 2.$$

[0254] FIG. 35 depicts a perspective cross-sectional view of open area 266 of membrane support 228. Open area 266 includes top portion 270, middle portion 274, and bottom portion 272. A length of middle portion 274 may less than a length of top portion 270 and a length bottom portion 272. Thus, an hourglass shaped opening is formed.

[0255] In a membrane-detection system, a fluid and/or sample in the detection region of the cartridge may be treated with a light. Interaction of the light with the fluid and/or sample may allow the analyte to be detected. Light from one or more light sources may shine on or in at least the detection region of a cartridge, such as the portion of the membrane where the fluid and/or sample is retained. The light may allow a signal from the retained fluid and/or sample to be detected. When light shines on a membrane surface, some of the light may be reflected. Areas proximate the detection region may also reflect some of the light that shines on a sample. Light reflecting from the membrane surface and/or membrane support may interfere with obtaining an accurate reading from the detector and so it may be advantageous to optically couple an anti-reflective material to the membrane and/or the membrane support.

[0256] In some embodiments, an anti-reflective material is optically coupled to the membrane and/or the membrane support. Alternatively, an anti-reflective material may be a coating on a surface of the membrane and/or membrane support. For example a black coating on a surface of the membrane and/or membrane support may act as an anti-reflective coating.

[0257] In certain embodiments, a portion of the membrane and/or membrane support may be made of an anti-reflective material. The anti-reflective material may be positioned above or below a membrane. An anti-reflective material may inhibit the reflection of light applied to analytes retained in or on the membrane. The anti-reflective material may absorb one or more wavelengths of light that are emitted by an analyte of interest. The anti-reflective material may improve the contrast of an image of at least a portion of the analyte retained in or on the membrane by inhibiting reflection of light.

[0258] In some embodiments, materials that form the components of the cartridge control flow of fluids through the cartridge. In some embodiments, hydrophilic material is coupled to the membrane and/or membrane support. Alternatively, hydrophilic material may be a coating on a surface of a membrane and/or membrane support. In certain embodiments, a portion of the membrane and/or membrane support is made from hydrophilic material. Hydrophilic material may enhance flow of a fluid through the membrane. Hydrophilic material may reduce the formation of air bubbles across the membrane and membrane support and/or inhibit nonspecific binding of analytes. Hydrophilic material may attract or have an affinity for aqueous fluids flowing through the membrane. Hydrophilic material may be positioned downstream of the membrane.

[0259] In some embodiments, hydrophobic material is positioned in or on the cartridge. Hydrophobic material may repel aqueous fluid away from surfaces of the cartridge and cause the fluid to flow towards the membrane. For example, positioning a top member above the membrane forms a cavity between the top member and the membrane. Hydrophobic material may be coupled to the top member. The hydrophobic material may be a coating on a surface of the top member, and/or the hydrophobic material may form a portion of the top member. As an aqueous sample or fluid enters the cavity, it is repelled away from the hydrophobic top member and flows towards the membrane.

[0260] A membrane-based detection system may be used alone or in combination with a particle-based detection system. In some embodiments, a particle-based detection system includes a supporting member with one or more cavities. One or more particles may be positioned in the cavities of the supporting member. In some embodiments, a particle-based detection system detects one or more analytes simultaneously using reactive particles that interact with the analytes.

[0261] In a particle-based detection system, a particle may produce a signal in the presence of an analyte. Particles may produce optical (e.g., absorbance or reflectance) or fluorescence/phosphorescent signals upon exposure to the analyte. Particles include, but are not limited to, functionalized polymeric beads, agarose beads, dextrose beads, polyacrylamide beads, control pore glass beads, metal oxides particles (e.g., silicon dioxide (SiO₂) or aluminum oxides (Al₂O₃)), polymer thin films, metal quantum particles (e.g., silver, gold, and/or platinum), and semiconductor quantum particles (e.g., Si, Ge, and/or GaAs).

[0262] The particles may include a receptor molecule coupled to a polymeric bead. The receptors, in some embodiments, are chosen for interacting with analytes. This interaction may take the form of a binding/association of the receptors with the analytes. A particle, in some embodiments, possesses both the ability to bind the analyte of interest and to create a modulated signal. The particle may include receptor molecules, which possess the ability to bind the analyte of interest and to create a modulated signal. Alternatively, the particle may include receptor molecules and indicators. The receptor molecule may possess the ability to bind to an analyte of interest. Upon binding the analyte of interest, the receptor molecule may cause the indicator molecule to produce the modulated signal. The receptor molecules may be naturally occurring or synthetic receptors formed by rational design or combinatorial methods. Natural receptors include, but are not limited to, DNA, RNA, proteins, enzymes, oligopeptides, antigens, and antibodies. Either natural or synthetic receptors may be chosen for their ability to bind to the analyte molecules in a specific manner.

[0263] Some particle-based detection systems and particles for use in particle-based detection systems are described U.S. patent application Ser. No. 09/616,731; U.S. Application Publication Nos.: 20020160363; 20020064422; 20040053322; 20030186228; 20020197622; 20040029259; 20050136548; and 20050214863; and U.S. Pat. Nos. 6,680,206; 6,602,702; 6,589,779; 6,649,403; 6,713,298; and 6,908,770.

[0264] In some embodiments, components necessary to obtain and assist in the analysis of a fluid and/or sample are included in a single package as a kit. In some embodiments, a package includes a cartridge, a sample collection device (e.g., a lancet, a syringe, or a needle), and one or more disinfectant

wipes. Disinfectant wipes may be used prior to using the sample collection device to draw a sample from a person. A disinfectant wipe may also be used by a user to wipe portions of the analyte-detection system before or after sample analysis. Packaging a cartridge and a sample collection device together may make collection and analysis of samples easier for an operator. Packaging a cartridge and a sample collection device together may inhibit contaminants from entering the cartridge and the sample collection device.

[0265] A package may be sealed to inhibit entrance of air (e.g. vacuum sealed). A package may be formed from a material that has at least one of the following properties: is water-proof, is water resistant, controls static electricity, kills microbes that enter the package, blocks sunlight, and blocks UV light. Materials that have these properties include polymeric materials or metal foils. A package may have a positive pressure to protect items in the package. Insulating materials, such as polyurethane or bubble wrap, may be placed inside a package to protect items in the package.

[0266] It may be desirable for the analyte-detection cartridge and/or system to include a control to ensure that the cartridge and/or system are operating correctly. Long storage times and/or less than ideal storage facilities may damage and/or affect the quality of the cartridge and/or components of the cartridge.

[0267] In some embodiments, it is desirable to check the fluids and/or reagents stored in the cartridge. A particle larger than cells to be detected or other particles in the sensor array may be placed in a detection system as a control analyte. For example, a control analyte includes any type of particle previously described, including quantum particles or dots. Control analytes may allow assessment of a cartridge and/or equipment used in conjunction with the cartridge, such as, but not limited to, light sources, detectors, analyzers, and/or computer systems. The control analyte may produce a result within a selected range and/or produce a result substantially similar to an expected result from a selected analyte.

[0268] In some embodiments a control analyte is a control particle. A control particle may be produced by coupling a known analyte to a particle. Reagents passing over the detection system may interact with the sample and the control particle. When an image of the detection system is captured the control particle is used to determine if the cartridge is functioning properly. For example, if a control particle is not detected, the quality of the reagents may be determined to be poor and the cartridge and assay discarded. In some embodiments, a control particle is distinguishable from other matter in the detection system due to the size of the control particle.

[0269] In some embodiments, a control analyte is stored in or on the cartridge. For example, a bead containing a known analyte may be designed to produce a predetermined signal. A weak or non-existent signal from the control analyte may indicate an improperly functioning cartridge.

[0270] In certain embodiments, a cartridge control system may be coupled to, positioned in, positioned on or integrated in the cartridge. The cartridge-control system may include, but is not limited to, one or more control analytes, one or more buffer solutions, and one or more reagent pads containing a dried predetermined analyte. In some embodiments, the cartridge-control system includes one or more fluid packages. The fluid packages may include one or more control analytes one or more control solutions, and/or other reagents. Prior to analyzing a sample, a control solution may be released from the fluid packages and pass over detection system.

[0271] In some embodiments, the detection system includes a control-detection system and an analyte-detection system. The known or control analyte may be applied to the control-detection system and the sample may be applied to the analyte-detection system. If the known analyte is captured by the control-detection system and a predetermined signal is produced, the cartridge is considered to be operating properly. If the known analyte passes through the control-detection system but does not produce an appropriate signal, it may indicate that the cartridge is not working properly (e.g., due to improper storage and/or age of the cartridge). Improperly working cartridges may be discarded prior to deposition of a sample on the cartridge. Once the quality of the cartridge has been confirmed, the sample is analyzed for analytes.

[0272] In some embodiments, a single detection system may be used to analyze the control analyte and the sample analytes. For example, if the known analyte is detectable in a detection system, the detection system may then be washed (e.g., laterally washing matter off the surface and/or back washing matter off the surface) to remove the known analyte from the detection system. After cleaning the detection system, a sample may be introduced to the detection system and a sample analysis performed.

[0273] In some embodiments, a detection system may be washed prior to use with fluid from a fluid delivery system. For example, a fluid package is coupled via a channel to a side or bottom surface of the detection system. Fluid from the fluid package washes the detection system such that the wash fluid, and any matter contained in the wash fluid, passes into an outlet channel of the detection region and into a waste region.

[0274] In some embodiments, an analyte-detection system is used with different cartridges to detect a plurality of analytes. The analyte-detection system may include a housing. The housing may include a slot for receiving a cartridge. In some embodiments, the housing includes an optical platform and/or an analyzer.

[0275] In some embodiments, an analyte-detection system may include an analyzer (e.g., a computer system). The analyzer may analyze images and/or control the one or more components of the analyte-detection system. The analyzer may be coupled to the housing and/or an optical platform of the analyte-detection system. The analyzer and/or analyte-detection system may include a display to show images produced by the detector. The analyzer and/or analyte-detection system may include a temperature controller. A temperature controller may control temperatures of or around the housing or components of the analyte-detection system.

[0276] The analyte-detection system may include a cartridge positioning system. In some embodiments, the cartridge positioning system is included in a housing of the analyte-detection system. The cartridge positioning system may automatically position the cartridge so that it is optically coupled to one or more light sources and/or one or more detectors. In some embodiments, one or more detectors and/or one or more light sources are coupled or directly attached to an optical platform.

[0277] One or more detectors may include, but are not limited to, a CCD detector, a CMOS detector, a camera, a microscope, or a digital detector. One or more detectors may detect one or more signals from an analyte. For example, a CMOS detector may be used for detection in membrane-based detection systems or for quantitative measurements while a CCD camera detector may be used for detection in particle-based detection systems. A signal may be repre-

sented by one or more wavelengths of light absorbed by: the analyte; matter retained on a membrane; a fluorophore; a particle, or combinations thereof. A signal may be represented by the fluorescence of: the analyte; matter retained on a membrane; a fluorophore; a particle; or combinations thereof. The detector may transform the signal to one or more images. The images may be of: one or more analytes in one or more fluids; samples retained on or in one or more membranes; one or more particles of a detection system; or combinations thereof.

[0278] In certain embodiments, a monochromatic detector may be used. When a monochromatic detector is used with multiple fluorophores and excitation sources, one or more filters may be used to isolate light emitted in a predetermined spectrum. For example, a green filter may be used to isolate the light emitted from the green fluorophore, and thus an image of the detection system may only include material that emits green light. A red filter may be used to isolate light emitted from a red fluorophore.

[0279] In some embodiments, one or more light sources may emit light of different wavelengths. For example, a light source may be capable of emitting two different wavelengths of light. Different wavelengths of lights may enhance detection of various types of analytes. In certain embodiments, different assays require different exposure times when images of the detection systems are obtained. An exposure time from approximately 1-5 seconds may be used.

[0280] In some embodiments, two light sources (e.g., blue and red LED light sources) and one or more detectors may be used to assist in detection of an analyte in a fluid and/or sample. Each light source may emit light at a different wavelength. For example, two light sources may be included in an optical platform and different combinations of light sources may be used to detect different analytes. Blue and red light sources may be used for CD4 cell assays, *E. coli* assays, β -galactosidase assay (β G) assays, and cell based assays. A blue light source may be used for CRP, tumor necrosis factor- α (TNF- α), and BG assays. A red light source may be used for interleukin-6 (IL-6) assays.

[0281] In some embodiments, an analyte-detection system includes several different lenses for the detection of different analytes. More than one lens may be used in the detection of some analytes. The lenses may be included in an optical platform and/or as part of a detector. Lenses of different magnification levels may be used in the analysis of one or more analytes. Lens magnification levels may include, but are not limited, 4 \times , 10 \times , and/or 20 \times . For example, a 10 \times lens may be used for CD4 assays, while a 4 \times lens may be used for CRP, TNF- α , and IL-6 assays. Alternatively, a 4 \times lens and a 10 \times lens are used in the detection of *E. coli* and/or β G assays.

[0282] In some embodiments, fiber optic cables are coupled to a detection system to facilitate image capturing. In certain embodiments, fiber optic cables are coupled to a particle-based membrane detection system to facilitate analyte-detection and reduce the need to adjust magnification between detection regions.

[0283] In some embodiments, an analyte-detection system includes a motor coupled to a lens and/or a detector. The motor may be coupled to the housing, the optical platform and/or a detector of the analyte-detection system. A motor may move the lens and/or the detector in a direction perpendicular to the plane the cartridge is positioned in, or the z-axis. Moving the lens and/or the detector vertically along the z-axis may focus the image of the detection region.

[0284] In some embodiments, a cartridge is coupled to a motor, actuator, or a cartridge positioning system designed to move the cartridge in the z-direction to focus an image of the detection region. A cartridge may be moved to allow more than one image of analytes to be captured in more than one detection system. For example, a cartridge contains more than one detection region. The area of interest in the detection systems may be too large to be captured with one image, thus the cartridge may be moved horizontally or in any direction along the x-y plane to obtain images of the desired areas.

[0285] FIG. 36 depicts a cartridge positioned in an analyte-detection system. Analyte-detection system 280 includes cartridge 100, housing 281 and optical platform 282. Optical platform 282 includes detector 284, light sources 286, 288, lenses 290, 292, 294, 296 and filters 298, 300, 302. Cartridge 100 may be positioned automatically and/or manually in housing 281. Light 304 (e.g., a white light) from light source 286 may be collimated with lens 290, filtered to a desired wavelength using filter 298 (e.g., filtered to a wavelength in a blue portion of visible light), and directed in or on a detection system positioned in detection region 108 of cartridge 100. In some embodiments, light from a light source may enter the cartridge at an angle. For example, the light source may be positioned at a 45° angle with respect to the detector and/or the cartridge. Filter 298 (e.g., excitation filters and/or clean-up filters) may be used to narrow excitations from light emitting diodes and/or other light sources. For example, filter 298 may be a D467/20x filter capable of filtering light to a wavelength ranging from about 450 nm to about 480 nm (e.g., 457 nm to about 477 nm). Filter 300 may be a 635/20x filter capable of filtering light to a wavelength ranging from about 625 nm to about 645 nm.

[0286] After light is directed into detection region 108, light 306 (e.g., signal) produced from interaction of the analyte with the sample may then be obtained using detector 284. The signal may be transformed into an image representing the desired analyte. In some embodiments, the image represents a membrane of the detection system and/or one or more analytes in the fluid and/or sample. Detector 284 includes, but is not limited to, a digital detector, a CMOS camera, or a CCD device. In some embodiments, moving the optical platform along the axis perpendicular to the cartridge while the cartridge is held static allows images of the cartridge to be brought into focus for the detector. Emission filter 302 may be used with detector 284. For example, light 306 reflected from the detection region 108 passes through lens 294 and/or an emission filter 302. Lens 296 is used to collimate light 306 from detection region 108 and/or focus the light from the detection region to detector 284. Emission filter 302 may be a dual band emission filter that allows transmission between about 504 nm and about 569 nm and between about 670 nm and about 822 nm.

[0287] Next, light 308 from light source 288 is collimated with a lens 292, filtered to a desired wavelength with filter 300, and focused on a sample. Emitted light 310 produced by interaction of the analyte with the sample and emitted from detection region 108 passes through lens 294 and/or emission filter 302 and is collimated with lens 296 to detector 284. Detector 284 obtains the signal from illumination of detection region 108 with light source 288. Emitted light 310 is transformed into an image representing an image of the detection region. It should be understood that additional light sources (e.g., a third light source, a fourth light source, a fifth light source, etc.) may also be used. Signals produced from the

detection region may then be processed to produce images of a portion of the detection region (e.g., a portion of a membrane) and/or of analytes present in the sample. In some embodiments, an analyzer determines the identity and/or presence of the analytes.

[0288] FIG. 37 depicts an alternative arrangement for an analyte-detection system 280. Optical platform 282 includes light sources 286, 288. Light sources 286, 288 emit light in a range from about 460 nm to about 480 nm, from about 465 nm to about 475 nm, or from about 460 nm to about 470 nm. During use, detection region 108 of cartridge 100 may be positioned automatically or manually in housing 281. Detection region 108 contains one or more detection systems (e.g., a membrane-based detection system and/or a particle-base detection system). The detection system includes at least one sample and at least one visualization agent. Light 304 from first light source 286 is collimated with lens 290, filtered to a desired wavelength using filter 298, reflected 90 degrees by dichroic mirror 312, and focused on a detection system in detection region 108 with lens 294. In some embodiments, the dichroic mirror is a combination of dichroic mirrors. The dichroic mirror may include one or more reflection bands and/or one or more transmission bands. For example, dichroic mirror 312 may be a Z502RDC long pass dichroic mirror, which is a dual band dichroic mirror having 2 reflection bands and 2 transmission bands. One reflection band of a dichroic mirror may reflect light at a wavelength ranging from about 463 nm to about 483 nm and transmit light ranging from about 502 nm to about 587 nm. A second reflection band of the dichroic mirror may reflect light at a wavelength ranging from 603 nm to about 637 nm and transmit light at a wavelength ranging from about 656 nm to about 827 nm.

[0289] Light 306 reflected and/or emitted from detection region 108 passes through lens 294, is filtered to predetermined wavelengths with filter 302 (e.g., a dual band emission filter), collimated with lens 296, and processed by detector 284 to produce an image of the detected analytes.

[0290] Light 308 from second light source 288 is collimated with lens 292, filtered to a desired wavelength with filter 300. Filter 300 is a different filter than filter 298, thus light 308 has a different wavelength than light 304. Filtered light 308 is reflected 90 degrees by dichroic mirror 314, reflected 90 degrees by dichroic mirror 312, and focused on or in detection region 108 using lens 294. Light 310 reflected and/or emitted from detection system 108 passes through lens 294, passes through dichroic mirror 312, is filtered to predetermined wavelengths with filter 302, is collimated by lens 296, and processed by detector 284 to produce an image of the detected analytes. Filter 302 may be a dual band emission filter capable of filtering light at two different ranges of wavelengths (e.g., a first wavelength from about 504 nm to about 569 nm and a second wavelength from about 607 nm to 822 nm).

[0291] The signal obtained by detector 284 may then be analyzed (e.g. using an analyzer) to determine the presence and/or identity of analytes in the detection region. Any number of light sources may be used in a similar manner as described above. It may be desirable to use a plurality of light sources to substantially simultaneously detect a plurality of analytes.

[0292] In some embodiments, a single light source with a beam splitter is used instead of multiple light sources. Using one excitation source may reduce costs. The single light source may excite two or more visualization agents applied to

matter captured on a membrane of a detection system of a cartridge. The emission of light from the detection system may be separated using one or more dichroic mirrors and one or more detectors.

[0293] FIG. 38 is a schematic of a cartridge positioned in an analyte-detection system with an optical platform that includes a single light source. Analyte-detection system 280 includes cartridge 100, housing 281, and optical platform 282. Optical platform 282 includes detectors 284, 316, light source 286, lenses 290, 294, 296, 318, filters 302, 320, dichroic mirrors 312, 314 and shutter 322.

[0294] Light 304 from single source 286 is collimated with lens 290, passed through shutter 322, reflected 90 degrees by dichroic mirror 312, and focused on detection region 108 of cartridge 100 with lens 294. Shutter 322 is positioned between lens 290 and dichroic mirror 312. Shutter 322 may block light from shining on detection region 108 and/or cartridge 100. Light 306 reflected and/or emitted from a detection system of detection region 108 may pass through lens 294, dichroic mirrors 312, 314, filter 302, and lens 296 where light 306 is collimated onto detector 284. A portion of light 306, depicted as light 306', may be reflected using dichroic mirror 314, pass through filter 320 (e.g., a dual band emission filter), and lens 318 where light 306' is collimated onto detector 316.

[0295] In some embodiments, an actuator is used to move a series of different emission filters into the path of light entering a detector. The ability to use different emission filters allows more than one signal from the detection region of the cartridge to be analyzed by one detector. The use of one detector and more than one filter may enhance the sensitivity of a test process, allowing less sample to be used for an analysis of multiple analytes. Determination of the appropriate emission filters to position in front of the detection system may be based on data obtained from a barcode located on the cartridge.

[0296] FIG. 39A is a schematic diagram of a cartridge positioned in an analyte-detection system that includes an optical platform equipped with an actuator. The actuator is designed to position a series of filters in front of a detector. Analyte-detection system 280 includes cartridge 100, housing 281, and optical platform 282. Optical platform 282 includes detector 284, light source 286, lenses 290, 294, 296, dichroic mirror 312, shutter 322, filter holder 324, filters 302, 320, and actuator 326. Light 304 from light source 286 is collimated with lens 290, passed through shutter 322, reflected 90 degrees by dichroic mirror 312, and focused onto detection region 108 of cartridge 100 with lens 294. Light 306 reflected and/or emitted from a detection region 108 may pass through lens 294, pass through dichroic mirror 312, pass through filter 302 or filter 320 positioned in filter holder 324, and lens 296 where light 306 is collimated onto detector 284. Filter holder 324 may include additional emission filters depending on the analyte to be analyzed. Filter holder 324 is coupled to actuator 326, which is designed to move filter holder 324. Actuator 326 may move filter holder 324 based on a signal from detector 284 and/or an analyzer of analyte-detection system 280. Filter holder 324 may be positioned between cartridge 100 and detector 284. In some embodiments, actuator 326 may move filter holder 324 such that filter 320 may be positioned between detector 284 and detection region 108 such that light 306 may pass filter 320 and into detector 284, as shown in FIG. 39B, allowing analysis of the detection region using a different wavelength of light. The

filter light (e.g., filtered signal) may then be analyzed in the detector to produce an image and/or data of analytes in the fluid and/or sample. A plurality of images and/or data from the fluid and/or sample may be obtained using a plurality of emission filters placed sequentially in front of the detector.

[0297] Analyte-detection systems described herein may be used to identify the presence of a plurality of analytes in a sample. Analyte-detection systems may be designed for detection of one or more specific analytes (e.g., cellular components, proteins, or pathogens such as viruses, bacteria, fungi or parasites, or combinations thereof) typically associated with various infections, diseases, illnesses, and/or syndromes. Examples of diseases, illnesses, viruses and syndromes include, but are not limited to, AIDS, malaria, heart disease, atherosclerosis, cancer, tuberculosis, mononucleosis, syphilis, sickle-cell anemia, herpes virus, HIV, Good's syndrome, or Sjogren's syndrome. Examples of herpes viruses include, but are not limited to, Epstein-Barr virus (EBV), cytomegalovirus (CMV), herpes simplex viruses 1 and 2 (HSV1 and HSV2), varicella-zoster virus (VZV), Kaposi's sarcoma-related virus (HHV8), herpes lymphotropic virus (HHV6), and human herpes virus 7 (HHV7).

[0298] Analysis of human blood samples may allow for early detection of various diseases, illness, viruses and/or syndromes. For example, WBCs and RBCs may be separated and analyzed to determine specific diseases, illnesses, viruses, and/or syndromes. In some embodiments, WBCs are separated from RBCs and immunotyped to determine the total number of various cell types in a sample and/or their ratio relative to other cell types. A five-part WBC differential, which is part of a typical complete blood count, may be used for general illness assessment. A five part WBC differential may sort out results based on counts of various white blood cells in various classes of diseases and may be used to diagnose viral, bacterial, allergic and immune diseases.

[0299] Samples may be analyzed by characterizing one or more components of a blood sample, including the fluid component of whole blood, such as serum or plasma. Samples may also be analyzed by characterizing one or more solid components of a blood sample. Solid components of a blood sample may include, but are not limited to, blood cells, platelets, or pathogenic organisms (e.g., bacteria, viruses, fungi, or blood-borne parasites).

[0300] In some embodiments, the cellular components of a sample may be characterized by detecting the presence and/or expression levels of one more molecular groups (e.g., polypeptides, polynucleotides, carbohydrates, lipids) typically known to be associated or correlated with a specific trait for which the test is being performed. For example, a blood sample may be collected to measure the number of one or more specific cell types present in the sample (commonly referred to in the art as "cell counts"), and/or the ratio thereof with respect to one or more different cells types also present in the sample. Examples of the types of blood cells that may be detected in a blood sample include, but are not limited to, erythrocytes, lymphocytes (e.g., T cells and B cells), Natural Killer (NK)-cells, monocytes/macrophages, megakaryocytes, platelets, eosinophils, neutrophils, basophils or mast cells. In some embodiments, various sub-populations of specific cell types within a fluid sample are distinguished. For

example, the T cells present in a blood sample may be further categorized into helper (CD4+), cytotoxic (CD8+), memory (CD4/CD8 and/or CD45RO) or suppressor/regulatory (CD4 CD25±FOXP3+) T cells. Alternatively, B cells present in a blood sample may be further categorized into populations of immature, mature, activated, memory, or plasma cells, based on the immunoglobulin isotype expressed on the cell surface, and presence or absence of various additional proteins.

[0301] Table I summarizes the surface expression profile of a selection of non-limiting protein markers that may be used to classify the stage of B cell differentiation, where filled circles denote expression, open circles denote lack of expression, and partially filled circles denote partial or limited expression of the indicated surface marker. The presently described systems and methods are not limited to detecting the cell types disclosed in Table I. It should be understood, that the presently disclosed systems and methods may be suitably adapted to analyze most cell types and/or macromolecules present in a biological sample without departing from the spirit and scope of the presently described embodiments.

TABLE I

B cell stage	Surface Immunoglobulin isotype			Marker protein				
	IgM	IgG _A or Ig	IgD	CD23	1 P CA -	CD38	CD25	CD10
Pre B	○	○	○	○	○	●	○	○
Immature	●	○	○	○	○	○	○	○
Mature	●	○	●	●	○	○	○	○
Activated	●	●	○	●	○	○	●	●
Memory	○	●	○	○	○	○	○	○
Plasma cell	○	○	○	○	●	●	○	○

[0302] Analysis of a cellular composition of a sample may include detecting the presence of one or more "surface markers" known to be expressed on the surface of the population of cells of interest. Certain surface markers useful in the differential identification of cells in a sample (e.g., in particular cells involved in immune responses) and/or diseases are commonly referred to as "cluster of differentiation (CD)" antigens or CD markers, of which over 250 have been characterized. Many of the CD antigens may also be referred to by one or more alternative art-recognized terms. Table II lists several examples of CD antigens, and the cells in which they are expressed, that may be referred to using one or more alternative terms. The system of CD marker nomenclature is widely recognized by ordinary practitioners of the art. General guidance in the system of CD marker nomenclature, and the CD expression profiles of various cells may be found in most general immunology reference textbooks such as, for example, in IMMUNOLOGY, 4th Edition Ed. Roitt, Brostoff and Male chapter 28 and Appendix II (Mosby/Times Mirror International Publication 1998), or in IMMUNOBIOLOGY: THE IMMUNE SYSTEM IN HEALTH AND DISEASE, 5th Edition, Eds. Janeway et al. Appendices I-IV (Garland Publishing, Inc. 2001).

TABLE II

CD	Identity/function	Expression
CD3	T cell receptor (γ , δ , ϵ , 4, 1)	Thymocytes, T cells
CD4	MHC class II receptor	Thymocyte subsets, T helper cells, monocytes, macrophages
CD8	MHC class I receptor	Thymocytes subsets, cytotoxic T cells
CD10	Neutral endopeptidase/CAALA	T and B-cell precursors, activated B cells, granulocytes
CD 11a	Integrin α	Lymphocytes, granulocytes, monocytes and macrophages
CD11b	Integrin α	Myeloid and NK cells
CD13	Aminopeptidase N	Monocytes, granulocytes
CD 16	Fc γ R111A/B	Neutrophils, NK cells, macrophages
CD19	B cell function/activation	B-cells
CD20	Ca ²⁺ ion channel	B-cells
CD21	C3d and EBV receptor	Mature B cells
CD35	Complement receptor 1	Erythrocytes, B cells, monocytes, neutrophils, eosinophils
CD41	allb integrin	Platelets, megakaryocytes
CD45RO	Fibronectin type II	T-cell subsets, B-cell subsets, monocytes, macrophages
CD45RA	Fibronectin type II	B cells, T-cell subsets (naive T cells), monocytes
CD45RB	Fibronectin type II	T-cell subsets, B cells, monocytes, macrophages, granulocytes
CD56	NKH-1	NK cells

[0303] In some embodiments, the presently described analyte-detection systems and methods may be used to analyze blood samples on the basis of the expression profile or presence of one or more macromolecules (e.g., proteins, phosphoproteins, glycoproteins, polynucleotides, or variants or isoforms thereof) that are indicative or prognostic of certain pathological states. Types of analytes that may be useful diagnostic or prognostic indicators and whose plasma or cellular expression levels are correlated with various diseases, illnesses, viruses, and/or syndromes include, but are not limited to, chemokine receptor 5 (CCR5), viral DNA or RNA sequences, certain species of plasma RNA, interferon-gamma (IFN- γ), virus particles, early secreted antigenic target protein-6 (ESAT-6), culture filtered protein-10 (CFP-10), C-reactive protein (CRP), troponin-I, and TNF- α .

[0304] In some embodiments, an analyte-detection system may be used for prognostic tests for HIV seropositive patients. HIV infects CD4+ cells (e.g., certain populations of T helper cells, monocytes and macrophages) by binding to a co-receptor CCR5. The expression level of certain CCR5 variants in CD4+ cells has been shown to correlate with viral load and progression to AIDS. The presently described analyte-detection systems and methods may be used to, for example, monitor CCR5 expression in CD4+ cells in patient blood samples. This parameter may advantageously be measured simultaneously from a single sample with one or more measures of HIV viral load. In some embodiments, the tests described herein may further measure one or more blood parameters associated with other pathological situations in addition to, or alternatively to, HIV infection.

[0305] In certain embodiments, an analyte-detection system may be used to diagnose tuberculosis (TB). In some embodiments, an analyte-detection system may be used to detect reductions in systemic CD3+ and CD4+ cells that typically occur in TB patients. This parameter may be measured alone or in combination with the detection of one or more soluble proteins typically elevated in TB patients (such as IFN- γ), the mycobacterial proteins ESAT-6, CFP-10, or T cells populations that are reactive to ESAT-6 and CFP-10. Such applications may be particularly suited to certain point-

of-care settings and/or in resource scarce countries where HIV and TB comorbidity are common.

[0306] In some embodiments, an analyte-detection system as described herein may be used to diagnose viral infections in addition to HIV. Blood samples from both Epstein-Barr virus (EBV) and cytomegalovirus (CMV) infected patients exhibit increases in percentages of total T-cells, suppressor T-cells and activated HLA-DR+ T-cells when compared with healthy, uninfected people. Additionally, as seen in HIV infected patients, individuals infected with EBV and/or CMV typically display significantly decreased levels CD4+ T-cells as well as a decrease in the ratio of CD4/CD8 T cells. Blood samples from individuals infected with EBV may also exhibit elevated levels of NK cells.

[0307] The analyte-detection systems described herein may, in some embodiments, be adapted to readily, reproducibly, and cost effectively diagnose a variety of maladies endemic to geographic and/or economically disadvantaged regions. An example of such an application is point-of-care diagnosis of malaria in geographic areas such as, for example, Africa, Latin America, the Middle East, South and Southeast Asia, and China. Currently, reliable diagnosis of malaria is time consuming, labor intensive, and typically involves identifying erythrocytes harboring *Plasmodium* parasites. Identification of such cells is typically made by microscopic examination of uncoagulated Giemsa-stained blood samples, possibly in combination with one or more serological and/or molecular diagnostic tests (e.g., polymerase chain reaction), all of which require highly specialized equipment. In some embodiments, analyte-detection systems described herein may be used to detect one or more *Plasmodium*-specific antigens that include, but are not limited to, panmalarial antigen (PMA), histidine-rich protein 2 (HRP2) and parasite lactate dehydrogenase (pLDH) in a blood sample. In some embodiments, the analyte-detection systems presently described may be used to monitor one or more physiological parameters associated with malaria. For example, a portion of the hemoglobin from *Plasmodium*-parasitized erythrocytes forms lipidized pigment granules generally referred to as "hemozoin." Phagocytosed hemozoin impairs monocyte/macrophage and hence immune function, at least in part, by reducing the

surface expression of MHC class II, CD11c and CD54 in phagocytes. Additionally, low peripheral blood monocyte counts may be associated with patients with severe and complicated malaria. Analyte-detection systems described herein may be used to detect and monitor the presence and/or quantities of these physiological parameters associated with malaria.

[0308] In some embodiments, analyte-detection systems described herein may be used to diagnose Good's syndrome, an immunodeficiency disorder secondary to thymoma and characterized by deficiencies of cell-mediated immunity and T-cell lymphopenia.

[0309] In some embodiments, an analyte-detection system may be used to identify certain biological markers associated with increased susceptibility to various pathological conditions (e.g., cardiovascular disease, atherosclerosis, inflammation, and/or certain types of cancer). Inflammation has been identified as an underlying cause of atherosclerosis, a condition associated with the deposition of lipids on the lining of arteries that may progressively lead to serious vascular complications such as myocardial infarction (MI) and/or stroke. By measuring the concentration of certain proteins associated with inflammation (e.g., CRP) either alone or in conjunction with cellular profiles (e.g., WBC count), the presently described analyte-detection systems may be used to screen individuals at risk for heart attack, atherosclerosis, or other vascular diseases. Likewise, MI patients with elevated CRP levels or WBC counts are at higher risk for subsequent cardiovascular events. Diagnostic and prognostic tests that provide measurements for these two important biological parameters associated with inflammation and vascular disease may provide powerful diagnostic and prognostic insight, allowing healthcare providers to make timely and appropriate therapeutic interventions. For example, it is recognized by practitioners of the art that individuals having elevated WBC counts and blood CRP levels have a greater risk for heart disease than individuals having WBC counts and CRP levels within normal range.

[0310] A low peripheral monocyte count in individuals with high cholesterol is generally predictive of increase risk for developing atherosclerosis. The presently described analyte-detection systems may be readily and advantageously adapted to measure monocyte counts (CD13⁺CD14⁺CD45RA) associated with cardiac risk factors. Monocyte counts are also an important physiological parameter in subjects with hypercholesterolemia. Analyte-detection systems described herein may also be used to measure the amounts of other cardiac risk factors such as troponin I and/or TNF- α .

[0311] A percentage of CD8⁺ cells and a number of monocytes in blood have been associated with progressive encephalopathy (PE). PE is one of the most common complications of HIV infection in children. As antiretroviral drugs become more available, the number of children with PE has increased, thus it is desired to evaluate risk factors for PE. CD8 stained cells may be identified using an analyte-detection system to monitor the progress of PE.

[0312] An analyte-detection system for use in diagnostic and prognostic applications to specific pathologies, such as for example, those described above, may further allow a user of the system to readily identify characteristics in a sample that are associated with the malady. The analyte-detection system may include, for example, various receptor molecules (such as specific antibodies) that bind to cell surface markers (e.g., CD markers or other disease-associated molecules) or

any other analyte suspected to be present in a sample that allows rapid characterization of the sample. In some embodiments, one or more antibodies (e.g., monoclonal and/or polyclonal antibodies) that specifically recognize and bind to macromolecules expressed on the surface of cells (e.g., CD or other cell surface markers) may be used in an analyte-detection system.

[0313] While certain specific examples of monoclonal or polyclonal antibodies are set forth above, it will be readily understood by ordinary practitioners of the art that the presently described analyte-detection systems may be used, without limitation, in conjunction with any type of antibody that recognizes any antigen, including, but not limited to, commercially available antibodies or antibodies generated specifically for the purpose of performing the tests described herein. Monoclonal and Polyclonal antibody design, production and characterization are well-developed arts, and the methods used therein are widely known to ordinary practitioners of the art (see, e.g., "Antibodies: A Laboratory Manual," E. Howell and D. Lane, Cold Spring Harbor Laboratory, 1988). For example, a polyclonal antibody is prepared by immunizing an animal with an immunologically active composition including at least a portion of the macromolecule to which the desired antibody will be raised and collecting antiserum from that immunized animal. A wide range of animal species may be used for the production of antiserum. Examples of animals used for production of polyclonal antisera are rabbits, mice, rats, hamsters, horses, chickens, or guinea pigs.

[0314] A monoclonal antibody specific for a particular macromolecule can be readily prepared through use of well-known techniques such as those exemplified in U.S. Pat. No. 4,196,265, which is herein incorporated by reference. Typically, the technique involves first immunizing a suitable animal with a selected antigen (e.g., at least a portion of the macromolecule against which the desired antibody is to be raised) in a manner sufficient to provide an immune response. Rodents such as mice and rats are preferred species for the generation of monoclonal antibodies. An appropriate time after the animal is immunized, spleen cells from the animal are harvested and fused, in culture, with an immortalized myeloma cell line.

[0315] The fused spleen/myeloma cells (referred to as "hybridomas") are cultured in a selective culture medium that preferentially allows the survival of fused splenocytes. After the fused cells are separated from the mixture of non-fused parental cells, populations of B cell hybridomas are cultured by serial dilution into single-clones in microtiter plates, followed by testing the individual clonal supernatants for reactivity with the immunogen. The selected clones may then be propagated indefinitely to provide the monoclonal antibody of interest. In some embodiments, a membrane-based detection system for use in performing WBC counts on a blood sample may use one or more polyclonal or monoclonal antibodies that specifically recognize various cell types that constitute WBCs to visualize specific blood cells. Antibodies suitable for this purpose include, but are not limited to: anti-CD3; anti-CD4; anti-CD8; anti-CD16; anti-CD56; and/or anti-CD19 antibodies to specifically recognize: T cells; T helper cells and monocytes/macrophages; cytotoxic T cells; neutrophils, NK cells and macrophages; NK cells; and B cells, respectively.

[0316] In some embodiments, a membrane-based detection system is used to assess both CD4 cell count and CD4 cells as

a percentage of total lymphocytes from a blood sample for diagnosis, staging, and/or monitoring of infections and/or diseases. For example, samples having CD4 counts below 200 cells per microliter may indicate specific drug therapy intervention. In certain embodiments, comparing CD4 cell counts to CD8, CD3, and/or CD19 cell counts may be used to assess the ratio CD4⁺ T helper cells with respect to cytotoxic T cells, total circulating T cells, B cells, or combinations thereof.

[0317] In some embodiments, a sample, such as blood or diluted blood, is applied and/or transported to a membrane of a membrane-based detection system. The membrane may retain portions of the sample, while allowing other portions of the sample to pass through. For example, the membrane may be adapted to retain lymphocytes, while allowing other portions of the sample, such as water or red blood cells, to pass through.

[0318] A combination of visualization agents may be applied and/or transported to the membrane to allow a total number and/or different types of lymphocytes (e.g., T-cells, NK-cells, and/or B-cells) to be identified. One or more visualization agents may be added to the matter collected on a surface of the detection system. For example, visualization agents may allow the detection of anti-CD3, anti-CD4, anti-CD8, anti-CD16, anti-CD56 and anti-CD19 antibodies bound to their respective CD markers on the surface of target cells. In some embodiments, anti-CD2, anti-CD4, and anti-CD 19 antibodies may be coupled to the visualization agent directly. In some embodiments, the visualization agent may be coupled to a second macromolecule that specifically binds to and recognizes the antibody bound to the CD marker.

[0319] In some embodiments, a first visualization agent may be used to stain CD4⁺ cells present in a mixed population of cells. Additional, distinct visualization agents may then be used to stain the NK-cells, B-cells, and/or other T-cells in the mixed population. For example, a mixed population of cells in a sample may be stained with anti-CD4, anti-CD3, anti-CD56, and anti-CD19 antibodies to detect CD4⁺ T helper cells, total T-cells, NK-cells, and B-cells respectively.

[0320] In some embodiments, fluorescent dyes (e.g., AlexaFluor® dyes from Invitrogen Corporation; Carlsbad, Calif.) may be coupled to antibodies to form fluorophore-labeled antibodies. Use of fluorophore-labeled antibodies to visualize cells may facilitate assessment of the sample. One or more fluorescent dyes may be used to label one or more cell surface markers to facilitate assessment of a desired marker percentage relative to other markers (e.g., a percentage of CD4⁺ lymphocytes relative to other lymphocytes). An image of the cells stained by the first visualization agent may be provided and one or more additional images of cells stained by the additional visualization agents may be provided. The images may be compared and/or combined to determine the total number of lymphocytes and/or a number of a specific type of lymphocyte in or on the membrane. A detector optically coupled to at least a portion of the membrane may provide the images. An analyzer may automatically compare the images during use. For example, AlexaFluor® 488, which fluoresces green when exposed to light having a wavelength of 488 nm, may be used to visualize anti-CD3 antibodies bound to the surface of all T cells present in a sample. AlexaFluor® 647, which fluoresces red when exposed to light having a wavelength of 647 nm, may be used to visualize anti-CD4 bound to the surface of T helper cells and monocytes. In this way, at least three populations of cells (all T-cells stain red, T helper

cells stain red and green, the overlap of which shows as yellow, and monocytes which stain green) may be readily and simultaneously identified in a single sample.

[0321] In some embodiments, two fluorophores and two light sources are used to determine types of lymphocytes. The analyte-detection system depicted in FIG. 36-FIG. 39 may be used, for example, to determine type of lymphocytes. FIGS. 40A-40C depict representations of images collected using two fluorophores and two light sources. For example, a green fluorophore (e.g., AlexaFluor® 488) may be coupled to anti-CD4 antibodies of a sample. A red fluorophore (e.g., AlexaFluor® 647) may be coupled to the anti-CD56 antibodies, anti-CD3 antibodies, and anti-CD19 antibodies added to the sample. As discussed above and shown in Tables I and II, CD4 is expressed on the surface of T helper cells and monocytes, CD19 is expressed on the surface of B cells, CD56 is expressed on the surface of NK cells, and CD3 is expressed on T cells. Analysis of the samples captured on a membrane using two wavelengths of light may allow differentiation of the types of WBCs captured.

[0322] FIG. 40A depicts a representation of image 330 of green cells 332, 334 obtained by exciting the green fluorophore visualization agent with a light source, analyzing the signal generated by the excitation, and producing an image of the cells. Green cells 332, 334 represent CD4⁺ cells.

[0323] FIG. 40B depicts a representation of an image of red cells obtained by exciting the red fluorophore, analyzing the signal produced from excitation, and producing an image of red cells. Red cells 338, 340, and 342, visible in image 344, represent cells expressing CD3, CD19 and CD56 respectively.

[0324] In digital detector images, cells that exhibit both green and red light may be combined to emit yellow light. Thus, monocytes (e.g., cells that only emit green light) may be identified and isolated. Combining image 330 and image 344 creates image 346 that includes green cells 334, red cells 338, 340, 342, and yellow cells 348, as shown in FIG. 40C. Green cells 334 are representative of CD4⁺CD3⁻CD19⁻. Yellow cells 348 are representative of CD4⁺CD3⁺ T helper cells.

[0325] A total number of T-helper cells (cells that express CD4 and CD3 and stain yellow), a total number of lymphocytes (cells that express CD3, CD19 or CD56 and stain red), a total number of CD4 cells (cells that stain green), and a ratio of CD4 cells to a total number of lymphocytes may all be determined from the combination of images 330, 344, 346. A total number of lymphocytes may be obtained from the combined image, as depicted in image 346, since the cells may be identified and isolated (e.g., cells that only emit green light or only emit red light).

[0326] An absolute number of CD4⁺ T helper cells is the total number of yellow cells 348. A ratio of CD4⁺ T helper cells to the total number of cells may be calculated by dividing the total number of yellow cells 348 (CD4⁺CD3⁺) by red cells 338, 340, 342 (CD3⁺, CD16⁺, CD456⁺, or CD19⁺).

[0327] The ratio of T-helper cells to total lymphocytes may be important in determining the progression of diseases, such as HIV, and in the treatment and monitoring of other diseases. Although green and red fluorophores were described, fluorophores of any color may be used without limitation.

[0328] In some embodiments, use of one or more visualization agents allows identification of lymphocytes retained on a membrane of a membrane-based detection system. The lymphocytes may contain cell surface markers CD4, CD3, and CD19. Identification of CD4 and CD3 and on the surface

of cells identifies T-helper cells. FIGS. 41A-41D represent images of cells expressing CD4, CD3, and CD 19 markers in the presence of two excitation sources.

[0329] FIG. 41A depicts an image of cells obtained by excitation of a green fluorophore attached to cells expressing CD4. An excitation source may excite green fluorophores and a detector may analyze the signal produced during excitation and produce image 350 of green cells 332, 336.

[0330] FIG. 41B depicts an image of cells obtained by excitation of a red fluorophore attached to cells expressing CD3 or CD19. An excitation source excites red fluorophores bound to the cells and a detector analyzes the signal produced during excitation and produces image 352 of cells 340 containing CD19 and cells 354 containing CD3.

[0331] Image 350 may be combined with image 352 to produce image 356 in which green cells 336, red cells 354, 340 and yellow cells 358 are visible. The total number of lymphocytes may be obtained from the combined image of cells stained red, green or yellow, as depicted in FIG. 41C. The total number of T helper cells present on the membrane is identifiable by determining the number of cells that stain yellow (e.g., those cells expressing both CD3 and CD4).

[0332] In some embodiments, a filter allows a desired wavelength of light to pass from the detection system to the detector. For example, a filter only allows yellow light to pass, as depicted in FIG. 41D. Thus, T cells 358 may be identified from image 360 collected by the detector. Using a filter may facilitate identification of one or more types of lymphocytes and/or other types of matter.

[0333] While a system to identify T cell populations based on differential staining of CD3, CD4, and CD 19 markers on cells is described above, it is understood that any combination of CD markers may be used to identify one or more types of lymphocytes and/or total lymphocytes in a sample.

[0334] In some embodiments, all cells except a lymphocyte of interest may be stained. A white light image of the membrane may be provided. One or more additional images may be provided in which cells stained with one or more visualization agents are visible. The number of a specific lymphocyte population may be obtained by assessing the number of cells appearing in the first image (e.g., the white light image) but not appearing in the additional images (e.g., images in which only stained cells appear). For example, a sample containing lymphocytes may be retained on a membrane of an analyte-detection system. A first image at a selected wavelength of light of the retained cells is taken. One or more visualization agents may be applied to the retained cells. At least one of the visualization agents stains part of the retained cells, but does not stain CD4⁺ cells. A second image at one or more wavelengths different than the wavelength for the first image is taken. Such "negative selection" strategies may be employed to determine the number of cells that are depicted in the first image but are not depicted in the second image, to give the number of CD4⁺ lymphocytes. Such strategies may be particularly suited to applications where additional functional analyses are performed on the cell of interest. For example, it is known in the art that contacting certain CD markers (e.g., CD3, CD19) with certain antibodies (commonly referred to as "cross-linking antibodies") causes profound changes in cellular physiology. Therefore, the negative selection strategy outlined above may be useful when additional biological/functional analyses are to be performed on a particular cell type.

[0335] In some embodiments, cells expressing CD4 may be stained red and cells expressing CD45 may be stained green. In certain embodiments, cells with certain surface markers may stain brighter than cells without the surface markers. For example, stained CD45 cells may appear brighter than stained CD4⁺ cells. A percentage of CD4 to total lymphocytes may be determined from the ratio of CD4⁺ cells to brighter stained CD45 cells.

[0336] It may be desirable to stain various cell subtypes differentially to allow discrimination between various cell types even when the cells are stained with antibodies with the same color tag. For example, CD4⁺ monocyte population may be differentiated from the CD4⁺ lymphocyte population. Low and high intensity CD4⁺ cells may be extracted from images of the detection system obtained by a detector. Weakly stained CD4⁺ cells may then be stained with a CD14 stain that identifies weakly stained CD4⁺ cells as monocytes.

[0337] Similar principles may be applied to other subsets of the lymphocyte population. A difference in the staining of NK-cells, B cells, and T-cells due to the number of surface markers, antibody affinity, or antibody performance may identify a CD8 population. CD8 monitoring and/or a ratio of CD4 to CD8 cells may be important in providing information about the progression of certain diseases, such as, for example, HIV progression and AIDS.

[0338] It may be desirable to obtain a CD8 percentage and monocyte count from a sample. Monocytes may exhibit a weaker stain with CD4 antibodies, which allows monocytes to be distinguished from CD4 T-cells, which are characterized by a strong stain with CD antibodies.

[0339] Differences in surface marker concentrations on cells may provide a tool for discrimination between cells. In some diseases, cell morphology may be correlated with disease states. Images from assay screening may provide information about the assay and cell morphology and may provide additional information about the disease. For example, the malaria antibody may be localized on a part of the cell to allow a difference in intensity across a cell to be observed. This difference in intensity may provide information about the health of the patient.

[0340] Different subpopulations of cells may accept the same stain but emit light at different intensities and so the subpopulations may be differentiated. The antibody binding capacity for various surface antigens may be measured using methods generally known to ordinary practitioners of the art. For example, CD4⁺ T-cells bind about 50,000 antibody molecules. Protocols for assay development and image analysis can be defined based on the relative amount of antibodies molecules that various cells can bind. Often exposure times may be adjusted to further separate populations. For example, a total T-cell population may be identified with an anti-CD3 antibody. Even though CD3 cells are stained with the same color as NK-cells and B-cells, the populations can be determined based on the differential staining characterizing these cells. As the CD3 population becomes separated from the rest of the cell count (e.g., by increasing exposure time when taking the image), the percentage of CD8 cells may be determined by subtracting the number of CD4⁺ cells and CD3⁺ cells from the total CD3 cell count. In some embodiments, when cells are stained with anti-CD8 antibody, there exists a strong intensity differential to discriminate CD8 cells from other cells such as NK-cells and B-cells. The strong intensity may accentuate the differential seen in a single color containing CD8⁺ cytotoxic T-cells, NK-cells, and B-cells. A ratio of

CD8⁺ cells may be calculated by dividing the total number of CD3⁺ cells minus the total number of CD4⁺ cells and CD3⁺ cells by the total number of CD3⁺ cells.

[0341] An analyte-detection kit including at least one cartridge designed for performing a pre-determined analysis, a sample collection device and disinfectant wipes may be opened. In some embodiments, the cartridge, wipes, sample collection devices are individually obtained. In certain embodiments, the cartridge is checked for viability prior to use. In some embodiments, a portion of a human may be wiped with one of the disinfectant wipes and a blood sample may be obtained with the sample collection device. A portion of the collected sample may be deposited on or in a collection region of the cartridge. For example, a finger may be pricked with a lancet and a drop of blood transferred to the cartridge using disposable tubing, a pipette, or a fluid bulb. In some embodiments, the sample may be deposited directly onto a membrane of a membrane-detection system. After the sample is introduced into a collection region of a cartridge, the collection region may be capped or sealed with, for example, an adhesive strip, a rubber plug, or a cover.

[0342] In some embodiments, one or more reagents may be provided to the sample. For example, anti-coagulant and/or fixative may be added to the blood sample. Fixatives include, but are not limited to, paraformaldehyde, ethanol, sodium azide, colchicine, Cyto-Chex® (Streck, Inc., Omaha, Nebr.), and Cyto-Chex® BCT. In some embodiments, a reagent may be provided to the sample. The reagent may be mixed with the sample during or after collection of the sample. Alternatively, a reagent may be added to a sample after the sample is introduced into a cartridge. In certain embodiments, a reagent may be provided to the sample by, for example, one or more pumps, fluid packages, and/or reagent regions coupled to, positioned in, and/or positioned on a cartridge.

[0343] The cartridge may be positioned, automatically or manually, in a housing of the analyte-detection system. The cartridge may substantially contain all fluids used for the analysis.

[0344] In some embodiments, a check of the cartridge may be performed. For example, the cartridge includes one or more particles having the desired analyte to be determined. An image of the particles may be obtained by one of the detectors. Analysis of the image is performed to determine if the known analyte can be detected. If the known analyte is detected, the cartridge is deemed suitable for use. If the known analyte is not detected, the cartridge may be disposed of and a new cartridge obtained. In some embodiments, the new cartridge is obtained from the kit or a supply of cartridges.

[0345] At least a portion of the sample may be provided to a metered volume portion of the cartridge. In some embodiments, the sample may be drawn by capillary action into the metered volume portion. In certain embodiments, the sample may be delivered by a fluid delivery system disposed in or coupled to the cartridge. After the sample has filled the metered volume portion, a portion of the sample may travel toward an overflow reservoir. In some embodiments, the sample may not be measured.

[0346] A fluid delivery system that includes a reagent may be actuated. Flow of fluid from the fluid delivery system may push a metered volume of sample from the metered volume portion towards a detection region that includes one or more detection systems (e.g., a particle-based detection system and/or a membrane-based detection system). The reagent and

sample may combine during passage of the sample toward the one or more detection regions to form a sample/reagent mixture. A portion of the sample/reagent mixture flows through or is collected in the detection region. The remaining portion of sample/reagent mixture may flow over or through the detection region to a waste region of the cartridge.

[0347] In some embodiments, the fluid delivery system is not necessary to push the sample towards the detection region. Capillary forces may transport the sample towards the detection region. In some embodiments, capillary forces that transport the sample are enhanced with hydrophilic materials (e.g., plastic or glass) to coat a channel for aqueous samples. Certain portion of channels may include hydrophilic materials positioned proximate the collection region, in the metered volume chamber, and/or proximate the overflow reservoir to direct flow of aqueous samples through a cartridge.

[0348] In some embodiments, the sample may be drawn into a channel via negative pressure in the channel. For example, suction created by a passive valve or a negative pressure source may create negative pressure in a portion of a channel and draw fluids towards the detection region. In some embodiments, valves may be used to direct the flow of fluid and/or sample through the cartridge.

[0349] One or more additional fluid delivery systems may be actuated to release one or more additional fluids (e.g., additional PBS, water, or other buffers). One or more of the additional fluids may flow over or through one or more reagent regions (e.g., a reagent pad or through a channel containing reagents). One or more reagents (e.g., one or more antibodies or a visualization agent) in or on the reagent regions may be reconstituted by the additional fluids. The reconstituted reagents may be transported to the detection region of the cartridge. Transport of the reconstituted reagents may be accomplished by continued actuation of the fluid delivery systems or through other methods described herein. The reconstituted reagents may label and wash a portion of the sample collected in one or more detection regions of the cartridge (e.g., wash WBCs retained on a membrane).

[0350] Portions of a sample and/or fluids may be provided to a detection region in a cartridge sequentially, successively, or substantially simultaneously. In some embodiments, a portion of the sample moves towards a detection region as a portion of the fluid from the second fluid delivery system flows towards a reagent region. Fluid from the second fluid delivery system may reconstitute and/or collect one or more reagents from the reagent region and deliver the reagents to the detection region after the sample has passed through the detection region. The collected reagents may then be added to an analytes that have been collected by the detection region.

[0351] Valves (e.g., pinch valves) and/or vents may be used to regulate flow of the sample. For example, a valve proximate the collection region may inhibit additional sample from flowing towards the detection region. In some embodiments, one or more changes in elevation of a channel may inhibit the sample from entering other channels.

[0352] In some embodiments, a reagent (e.g., a visualization agent or one or more antibodies) may be directly added to the matter on a membrane of a membrane-based detection system. The sample may then be washed with fluid remaining in the first fluid delivery system or with the fluid from one or more of the fluid delivery systems.

[0353] In some embodiments, only one fluid delivery system is used. For example, one or more syringes may be at least partially coupled to, positioned in, or positioned on the car-

tridge. Each syringe may contain one or more fluids to be used during the analysis. The syringes may be actuated and the fluids delivered sequentially, successively, or substantially simultaneously to the collection region, the reagent regions and/or the detection region.

[0354] In some embodiments, analytes collected on a membrane of a membrane-detection system may be viewed through a viewing chamber of the membrane-detection system. Light sources may be activated and light may be directed towards the membrane-based detection system. Light may enter the membrane-detection system through a viewing chamber and/or a top layer of the membrane-detection system. A detector may collect a signal produced from interaction of light with one or more analytes in the detection region. In some embodiments, the detector may be optically aligned with the viewing chamber of the membrane to allow the membrane and/or detection region to be viewed by detector.

[0355] The detector processes the produced signal to produce images representative of the analytes collected by the detection system. Images may be obtained concurrently or simultaneously. Images may be analyzed and the analytes in the sample assessed.

[0356] The cartridge may then be removed from the analyzer and discarded. The above-described method may then be repeated for the next sample. In certain embodiments, portions of the analyzer may be disinfected between samples. In some embodiments, the cartridge is self-contained such that all fluids remain in the cartridge and the analyzer may not need to be disinfected.

[0357] Interaction of a sample with light produces a signal that is received by the detector. The detector may produce images from the signal. Images may be analyzed by an analyzer (e.g., automatically with a computer or manually by a human) to determine the analytes present in the sample.

[0358] A third fluid delivery system may be activated to allow a wash solution to flow through or over the detection region. The detection region may be washed repeatedly to clear the detection region and prepare for additional use.

[0359] The first fluid delivery system may be actuated, or a fourth fluid delivery system may be used, to push a second portion of sample towards the membrane. The analysis may be repeated to determine different and/or duplicate sample analysis.

[0360] The procedure may be repeated as necessary to obtain the needed data. Additional samples may also be obtained and used. In some embodiments, one or more membranes may be used in a membrane-based detection system. After all analyses have been completed, the cartridge may be properly discarded.

[0361] In some embodiments, an analyte-detection system may be used to test for two or more analytes. The first and second analytes may include a wide range of cellular and/or chemical/biochemical components. Chemical/biochemical components may include, but are not limited to, electrolytes, proteins, nucleic acids (e.g., DNA and/or RNA), steroids and other drugs. In certain embodiments, an analyte-detection system may be designed to test for indications of cancer (e.g., types of cancerous cells and/or levels of related biochemicals) as well as one or more diseases. For example, an analyte-detection system may be designed to test for cervical cancer and sexually transmitted diseases.

[0362] In some embodiments, one or more cellular components of blood and/or one or more proteins may be assessed concurrently in an analyte-detection system including par-

ticle- and/or membrane-based detection systems coupled to one or more fluid flow systems. The proteins may include protein cardiac biomarkers. Protein cardiac biomarker targets may include, but are not limited to, proteins related to risk assessment, prognosis, and/or diagnosis. Protein cardiac biomarker targets related to necrosis, thrombosis, plaque rupture, endothelial dysfunction, inflammation, neurohormone activation, ischemia, arrhythmias, and/or other conditions may be assessed. Protein cardiac biomarker targets assessed by particle-based detection systems may include, but are not limited to, cardiac troponin T (cTNT), cardiac troponin I (cTNI), myoglobin (MYO), fatty acid binding protein (FABP), myeloperoxidase (MPO), plasminogen activator inhibitor-1 (PM-1), tissue factor, soluble CD40 ligand (sCD40L), von Willebrand factor (vWF), D-dimer, matrix metalloproteins (MMPs), pregnancy associated plasma protein (PAPP), placental growth factor (PlGF), soluble intercellular adhesion molecules (sICAM), P-selectin, CRP, high sensitivity C-reactive protein (hs-CRP), oxidized low-density lipoprotein (ox-LDL), monocyte chemoattractant protein-1 (MCP-1), interleukin-18 (IL-18), IL-6, TNF- α , B-type natriuretic peptide (BNP), norepinephrine (NE), ischemia modified albumin (IMA), free fatty acids (uFFA), and combinations thereof.

[0363] The cellular components may include cellular cardiac biomarkers. Cellular cardiac biomarkers may include, but are not limited to, white blood cells, circulating endothelial cells, platelets, and/or combinations or subsets thereof. In some embodiments, for example, a white blood cell subset may include lymphocytes. Identification of ESAT-6 and CFP-10 specific T-cells may be desirable. ESAT-6 and CFP-10 may be tagged with a fluorophore and passed through a membrane of a detection system where they bind with T-cells. In certain embodiments, fluid is directed to a particle-based detection system after passage through the membrane, where the particle-based detection system includes a particle derivatized with anti-IFN γ .

[0364] Tests targeting CRP and WBCs are widely available in clinical settings; they are typically administered separately on different instruments. These tests may require large sample volumes, additional sample preparation steps, and longer assay times. In addition, the clinical instruments and methodologies currently used to complete these tests are not suitable for point of care testing, such as in the doctor's office, in an emergency room, or in an ambulance. The diagnostic and prognostic value of these biomarkers may be enhanced if these two tests could be administered concurrently on the same instrument, in a convenient, accurate and highly accessible manner.

[0365] In some embodiments, an analyte-detection system is used to analyze two or more analytes in a fluid and/or sample. A first analyte may be cellular matter and a second analyte may be a one or more protein components. For example, the first analyte may be WBCs and the second analyte may be CRP. A sample (e.g., whole blood) may be obtained using the methods described herein or other sampling techniques known in the art. A portion of the sample may be provided to a collection region of a multi-functional cartridge.

[0366] At least a portion of the sample may be provided to a metered volume portion of the cartridge. In some embodiments, the sample may be drawn by capillary action into the metered volume portion. In certain embodiments, the sample may be delivered to a metered volume portion using a fluid

delivery system. As the sample fills the metered volume portion, an excess portion of the sample may travel toward an overflow reservoir. The metered portion of the sample may be advanced toward one or more regions including, but not limited to, a particle-based detection system, a membrane-based detection system, a cell-lysing chamber, a processing chamber, a polymerase chain reaction chamber, or combinations of these regions. In some embodiments, a metered volume portion of the cartridge may not be necessary.

[0367] Portions of the sample may be provided to detection systems in the cartridge sequentially, successively, or substantially simultaneously through pathways (e.g., channels) described previously. In some embodiments, a portion of the sample may be provided to a membrane-based detection system, passed through the membrane-based detection system, and the remaining sample is provided to a particle-based detection system. In some embodiments, a portion of the sample may be provided to a particle-based detection system before a portion of the sample is provided to a membrane-based detection system. In certain embodiments, portions of the sample may be provided to a particle-based detection system and a membrane-based detection system via separate pathways (e.g. channels) substantially simultaneously. In some embodiments, a sample from a single collection region may be provided to two or more pathways. In certain embodiments, samples may be provided to two or more collection regions and processed independently. After the collection region is filled, the collection region may be capped or sealed with a cover. At least a portion of the sample may be delivered to a membrane-based detection system by methods including, but not limited to, activation of a fluid delivery system.

[0368] In some embodiments where the cartridge is designed for analysis of blood samples, one or more membranes may be used to achieve separation of various whole blood components. For example, after the whole blood sample is provided to the membrane, WBCs may remain on the surface of the membrane, while other components of the blood sample (e.g., RBCs and/or plasma) move through the membrane toward a waste reservoir or along one or more paths for further analysis. Cellular components (e.g., WBCs) on the surface of the membrane may be washed or otherwise treated or assessed (e.g., counted). In some embodiments, one or more reagents (e.g., one or more WBC-specific antibodies labeled with an indicator molecule) may be provided to the membrane by one or more fluid delivery systems. In certain embodiments, reagents provided to a sample may be filtered, reconstituted, or otherwise processed in a portion of the cartridge. The portion of the blood sample that passes through the membrane may be directed toward an additional membrane for filtering. For example, a second membrane may remove RBCs from the blood sample. In some embodiments, RBCs may be further processed (e.g., lysed or recovered) and assessed by polymerase chain reaction (PCR), hematocrit count/calculation, and/or other tests.

[0369] In some embodiments, a portion of the blood sample that is substantially free of particulate (e.g., cellular) components may be directed toward a particle-based detection system for further analysis. For example, plasma may be directed toward a particle-based detection system that includes particles designed to detect specific proteins in the plasma. For example, particles designed to detect CRP may include CRP-capturing antibodies coupled to the particles. In some embodiments, one or more reagents may be delivered to the particle-based detection system by mechanisms including,

but not limited to, fluid packages, reagent pads, or mini-pumps. In certain embodiments, a reagent delivered to a particle-based detection system may include one or more labeled antibodies. The amount and/or identity of the analytes may be assessed using an analyte-detection system. In some embodiments, the cartridge may be positioned, manually or automatically, to allow an analyte-detection system to analyze a membrane-based detection system. The cartridge may then be repositioned, manually or automatically, in the analyte-detection system to allow analytes in the particle-based detection system to be assessed.

[0370] A non-limiting example of a multi-functional detection system is set forth below. An analyte-detection system was used for the concurrent measurement of both CRP and WBCs. The analyte-detection system included a multi-functional cartridge. The cartridge included a particle-based membrane detection system and a membrane-based detection system. The membrane-based detection system was configured to capture and detect blood cells, while the particle-based detection system was configured to interact with blood proteins. The detection systems were each coupled to a fluid delivery system. The two detection systems shared a common computer. The computer controlled fluid delivery systems and optical components. The fluid delivery systems provided fluids for the analysis. The optical components assisted in microscopic evaluation of signals collected from the two detection systems.

[0371] The particle-based detection system of the cartridge was used to perform a CRP-specific immunoassay. The particle based detection system included porous agarose micro-particles positioned in a micro-etched array (3x3 array) of wells on a silicon wafer microchip. Three particles, coated with antibodies irrelevant to CRP, were used as negative controls. The other six particles were dedicated to CRP capture and detection. Rabbit CRP-specific antibodies were coupled to the particle to capture the CRP antigen. This level of particle redundancy increased the statistical significance and, hence, the precision and accuracy of the CRP measurements. AlexaFluor 488 labeled antibodies were employed to visualize the particle-captured protein.

[0372] A portion of the blood sample was introduced to the particle-based detection system, and the particles were washed with PBS. Low internal volumes of each particle (about 2 mL to about 30 mL, per bead) used in conjunction with high effective flow rates (1-5 mL/min) allowed for the completion of highly stringent washes (>5000 effective washes per minute). The wash efficiently reduced nonspecific binding of antigens and detecting antibody reagents to the particles.

[0373] After washing, an image of the particle array was acquired in the following manner. Using standard epi-illumination geometry, white light from a 100-W mercury lamp was collimated, passed through a filter to select the excitation wavelengths centered at 480 nm with a 40 nm spectral bandwidth, reflected by a dichroic mirror (505 nm long pass mirror), and focused onto the particle array using a 4x microscope objective (NA of about 0.13). The fluorescence from the particles was collected by the microscope objective, transmitted through the dichroic mirror, passed through an emission filter centered at 535 nm with a 50 nm spectral width and detected by a CCD camera. The image was digitally processed and analyzed, and the signal intensity converted for each particle into a quantitative CRP measurement with the

aid of a calibration curve. The time required to process the sample was approximately 12 minutes.

[0374] The particle-based detection region was washed with PBS and another image was acquired. Each assay of the sample was followed by a wash with PBS.

[0375] The particle-based CRP assay generally exhibited a detection range of at least 1 ng/mL up to 10,000 ng/mL. With the appropriate choice of assay conditions, use of particles coated with varying concentrations of capturing antibody, and/or use of sample dilution, the detection range for CRP was estimated to be expandable up to 100,000 ng/mL.

[0376] The above-described particle-based CRP assay was validated against a commercial high sensitivity-CRP enzyme limited immunosorbent assay (ELISA). CRP values from 9 human blood samples evaluated in parallel by ELISA and the particle-based method were determined to be in agreement with each other.

[0377] A portion anti-coagulated blood sample was fixed with 4% paraformaldehyde, and then incubated for 5 minutes with an AlexaFluore® 488 labeled anti-CD45 antibody specific for WBCs. Coagulation of blood may be inhibited by adding an anti-coagulating agent to the blood sample (e.g., heparin or ethylenediaminetetraacetic acid (EDTA)). The mixture was diluted with PBS and introduced to a membrane of the membrane-detection system with the use of an external peristaltic pump equipped with an injection valve. The membrane was a supported 13 mm track-etched polycarbonate membrane. Image acquisition was performed as described above for the particle-based detection system. Analysis of the scanning electron micrographs of the filtered whole blood revealed that RBCs, with roughly the same diameter as the WBCs, deformed and passed through the 3.0 micrometer pores of the membrane while WBCs were captured on the membrane. After removal of the RBCs, the WBCs were stained with anti-CD45 antibody. Two populations of cells were observed. One population of cells was brighter than the second population of cells captured on the membrane.

[0378] To evaluate the linearity and analytical range of the membrane WBC assay, increasing volumes of a CD45-stained whole blood suspension were delivered to the membrane-based detection system. Following a rinse with PBS, images of the WBCs on the membrane were captured at 3 different fields of view (FOV) on the membrane. A pixel analysis algorithm, as described in U.S. patent application Ser. No. 10/522,499, was applied to identify and count individual WBC based on size, shape, and fluorescence intensity thresholding within the image J environment. From the images, it was determined that the WBC counts increased in a linear fashion with an increasing volume of blood delivered to the flow cell. The coefficient of variation (CV) of the counts measured in different FOVs (intra-assay precision) was found to be within the range of 5% to 15%, and was dependent on the volume of blood delivered on the membrane. Optimal precision with the above-described cell structure was achieved for volumes of blood between 0.81 μ L and 14.3 μ L.

[0379] To evaluate the inter-assay precision of the WBC assay, the equivalent of 2.1 μ L of stained whole blood was delivered to the membrane-based detection system. For healthy donors with 5000 to 11,000 WBCs/ μ L, this volume of blood includes 10,500 to 23,100 WBCs. With the optical instrumentation described above, one FOV represented an area of 0.60 mm². Given that the total surface area of the membrane utilized for cell capture is 78.54 mm², the current membrane element was estimated to yield about 130 FOVs.

Consequently, while the entire sample volume yields 10,500 to 23,100 FOVs, the single FOV collected a fluorescence signature of about 80 to about 176 cells, assuming that the cells were evenly distributed across the entire membrane.

[0380] Images from 5 non-overlapping FOVs were captured to get the preliminary mean WBC count. The preliminary count was converted to an absolute count after application of a scaling factor that incorporated the volume of blood delivered to the flow cell, as well as the number of FOVs covering the membrane-based detection system onto which WBCs are captured. The experiment was repeated 5 times using different membrane-based detection systems of the same configuration. The inter-assay coefficient of variation of the counts from one membrane-based detection system to another membrane-based detection system was determined to be 4.3%.

[0381] Additionally, the WBC counts achieved by the membrane counting method were in agreement (95%) with those determined by flow cytometry. Flow cytometry requires a larger blood sample size (100 μ L) and an additional processing step to lyse the red blood cells. The excellent agreement between flow cytometry and membrane-based detection indicates that the assumption of even cell distribution on the membrane of the membrane-based detection system was accurate.

[0382] As shown by this example, an analyte-detection system that includes a particle-based detection system and a membrane-based detection system allows for enhanced CRP detection levels in whole blood and for separation, isolation and detection of white blood cells from whole blood.

[0383] Certain U.S. patents and U.S. patent applications have been incorporated by reference. The text of such U.S. patents and U.S. patent applications is, however, only incorporated by reference to the extent that no conflict exists between such text and the other statements and drawings set forth herein. In the event of such conflict, then any such conflicting text in such incorporated by reference U.S. patents and U.S. patent applications is specifically not incorporated by reference in this patent.

[0384] Referring to FIG. 42, LOC immunoassays are performed on porous agarose beads (~280 μ m) positioned in a micro-etched array of wells on a silicon chip. Each bead serves as its own independent self-contained micro-reactor. Here, analyte-specific capturing ligands (allergens or antibodies) are coupled to the beads via reductive amination. Consequently, the selectivity of each bead is determined by the specificity of the ligand that it hosts.

[0385] Referring to FIG. 43, the bead-loaded chip is sandwiched between two optically transparent polymethylmethacrylate inserts, packaged within a metal casing described as the "flow cell". The flow cell allows for microfluidic and optical access to the microchip and the associated beads.

[0386] Referring to FIG. 44, fluids are delivered via the top inlet of the flow cell, soaking evenly the beads located within the array. Unspent reagents are directed to a waste reservoir through the bottom drain. Images of fluorescent beads are captured with a digital video chip/charge-coupled device (CCD).

[0387] Referring to FIG. 45, an image of an array of micro-reactor beads is captured digitally. A dedicated macro measures the signal intensity of an area of interest (AOI) around each bead. The average signal intensity of each AOI is exported to a data spread sheet for further analysis to deter-

mine a positive versus a negative result or to provide a quantitative evaluation of an unknown sample by a comparison to a standard curve.

[0388] FIG. 46 shows immunoschematics of LOC-based total (A) and allergen-specific (B) human IgE assays.

[0389] FIG. 47 illustrates a typical result of the LOC-based assay for total IgE. Redundant ($\times 16$) beads coated with antibody specific for human IgE produce a fluorescent signal when exposed to 500 IU/mL of human IgE standard. In contrast, the non-specific signal developed on beads coupled to a control, rabbit antibody irrelevant to IgE, is non-detectable.

[0390] FIG. 48 is a dose-response curve for the LOC total human IgE assay. The LOC system provides a rapid, sensitive, and reliable assay for total serum IgE. The minimal sensitivity of this assay is estimated at 1.0 IU/mL.

[0391] Referring to FIG. 49, the capacity of the LOC system to accurately detect allergen-specific human IgE is evaluated using positive and negative control sera obtained from Hycor, Inc. Here, the system detects IgE specific for some of the allergens indicated, as well as total human IgE (A and B). When the system is challenged with IgE-negative serum no detectable signal is observed (C).

[0392] FIG. 50 illustrates a typical result of the allergen-specific LOC test using serum from a volunteer donor. Here, serum from donor UT001 tests positive for allergies to peanut, ragweed, mold, dust mites (p and f) and timothy grass. The same individual tests negative for IgE against cat and dog epithelia. Detection of total IgE is also demonstrated.

[0393] Referring to FIG. 51, validation studies of the LOC approach were performed using samples obtained from 7 volunteer donors from our laboratory. Serum samples were evaluated in parallel by LOC and ELISA (AlerCHEK, Inc.) methods. Negative and positive controls (not shown here) were used to demonstrate the specificity of the reactions and to set the threshold levels for signals indicative of a positive/negative. This table provides a comparison of the results achieved by the two methods. With such measurements, there is a close agreement between the two methods for the majority of the allergens tested. A question mark indicates a very low-level positive result; ND indicates an inconclusive test result.

[0394] Further details may be found in a U.S. Provisional Application 60/693,613, entitled "ANALYTE-DETECTION SYSTEMS AND METHODS INCLUDING SELF-CONTAINED CARTRIDGES WITH DETECTION SYSTEMS AND FLUID DELIVERY SYSTEMS," filed Jun. 24, 2005 and naming John T. McDevitt, Karri L. Ballard, Nicolaos J. Christodoulides, Pierre N. Floriano and Glennon W. Simmons as co-inventors, the entire contents of which are incorporated herein by reference. Subsequently, a PCT application was filed claiming priority to this provisional (International Application No. PCT/US2006/024603), which is also incorporated herein by reference in its entirety.

[0395] Further modifications and alternative embodiments of various aspects of the invention will be apparent to those skilled in the art in view of this description. Accordingly, this description is to be construed as illustrative only and is for the purpose of teaching those skilled in the art the general manner of carrying out the invention. It is to be understood that the forms of the invention shown and described herein are to be taken as the presently preferred embodiments. Elements and materials may be substituted for those illustrated and described herein, parts and processes may be reversed, and certain features of the invention may be utilized indepen-

dently, all as would be apparent to one skilled in the art after having the benefit of this description of the invention. Changes may be made in the elements described herein without departing from the spirit and scope of the invention as described in the following claims.

What is claimed is:

1. A method of detecting human or animal IgE in blood materials, the method comprising:

providing one or more beads at least partially contained within a microchip structure, the bead or beads coated with one or more isolating substances selected to bond to animal IgE;

exposing the bead or beads to a blood sample material containing animal IgE, such that the one or more isolating substances bond with the animal IgE;

applying a marker agent to the bead or beads, the marker agent selected to bind to the bonded animal IgE; and determining the presence of animal IgE on the bead or beads by detecting the marker agent.

2. The method of claim 1 wherein the microchip structure is contained within a removable cartridge, the method including inserting the removable cartridge into a corresponding slot of a blood analyzer.

3. The method of claim 2 wherein exposing the bead or beads to a blood sample material includes applying the blood sample material to a collection region of the cartridge, the collection region being coupled to the microchip structure such that the blood sample material flows to the microchip structure from the collection region.

4. The method of claim 2 further comprising storing the marker agent in the cartridge and delivering the marker agent to the microchip structure after exposing the bead or beads to the blood sample material.

5. The method of claim 2 further comprising, after detecting the marker agent, removing and disposing of the cartridge.

6. The method of claim 1 wherein the one or more beads comprises multiple beads coated with respective isolating substances, each isolating substance comprising an allergen or anti-IgE antibody selected to bond to a respective allergen-specific animal IgE.

7. The method of claim 6 wherein the provided beads include beads coated with different allergens from a selected panel of allergens, with at least one bead coated with each of the allergens of the panel.

8. The method of claim 7 wherein the panel of allergens comprise one or more of cat hair, dog hair, Timothy grass, Johnson grass, dust mite, ragweed, and mold.

9. The method of claim 7 wherein the panel of allergens comprise one or more of latex, cedar, fire ants, fleas, *candida albicans*, cotton, egg yolk, crab, coffee, lobster, and salmon.

10. The method of claim 1 wherein the agent contains a fluorophore.

11. The method of claim 10 wherein determining the presence of animal IgE comprises directing a light source toward the beads and detecting a fluorescent signal from the fluorophore in response to the light source.

12. The method of claim 11 wherein determining the presence of animal IgE further comprises correlating intensity of the detected signal with concentration of the IgE.

13. The method of claim 11 wherein the detected signal is captured digitally to produce an image of the one or more beads of the microchip to which antigen specific IgE is bound.

14. The method of claim 13 further comprising identifying from the image an antigen specific IgE antibody present in the blood.

15. The method of claim 1 wherein the beads comprise porous agarose beads.

16. The method of claim 1 wherein the isolating substance is a rabbit anti-human IgE that binds to human IgE.

17. The method of claim 1 wherein exposing the bead or beads to the blood sample material comprises applying a blood material sample of less than about 50 micro liters.

18. The method of claim 1 wherein the microchip structure defines an array of wells, the beads being disposed within the wells.

19. An allergen sensitivity analysis cartridge comprising a cartridge housing sized to be received into a blood analyzer, the housing defining a blood sample material collection region of the cartridge, the collection region being coupled to the microchip structure such that the blood sample material flows to the microchip structure from the collection region;

a microchip contained within the cartridge housing and hydraulically connected to the blood sample material collection region such that blood sample material deposited at the collection region flows to the microchip, the microchip containing one or more beads coated with one or more isolating substances selected to bond to animal IgE; and

a marker agent selected to bind with animal IgE and contained within a marker agent chamber of the cartridge, the cartridge housing defining a channel from the cavity to the microchip for exposure of the marker agent to the coated beads.

20. The cartridge of claim 19 wherein the one or more beads comprises multiple beads coated with respective isolating substances, each isolating substance comprising an allergen or anti-IgE antibody selected to bond to a respective allergen-specific animal IgE.

21. The cartridge of claim 19 wherein the beads include beads coated with different allergens from a selected panel of allergens, with at least one bead coated with each of the allergens of the panel.

22. The cartridge of claim 21 wherein the panel of allergens comprise one or more of cat hair, dog hair, Timothy grass, Johnson grass, dust mite, ragweed, and mold.

23. The cartridge of claim 21 wherein the panel of allergens comprise one or more of latex, cedar, fire ants, fleas, *candida albicans*, cotton, egg yolk, crab, coffee, lobster, and salmon.

24. The cartridge of claim 19 wherein the agent contains a fluorophore.

25. The cartridge of claim 19 wherein the beads comprise porous agarose beads.

26. The cartridge of claim 19 wherein the isolating substance is a rabbit anti-human IgE that binds to human IgE.

27. The cartridge of claim 19 wherein the microchip structure defines an array of wells, the beads being disposed within the wells.

28. The cartridge of claim 19 wherein the microchip is contained within a microchip chamber of the housing.

29. The cartridge of claim 19 wherein the microchip chamber is defined between two transparent walls of the cartridge housing.

30. The cartridge of claim 29 further comprising a waste reservoir to collect residual blood sample material and marker agent flowing from the microchip chamber.

31. The cartridge of claim 19 wherein the marker agent chamber is defined within a pouch exposed on an outer surface of the cartridge housing.

32. The cartridge of claim 19 further comprising a flush solution chamber containing a flush solution.

33. The cartridge of claim 32 wherein the flush solution chamber is defined within a pouch exposed on an outer surface of the cartridge housing.

34. A portable analyzer comprising:
an analyzer housing having a cartridge receptacle configured to receive a disposable analysis cartridge; and
the cartridge of claim 19.

35. The analyzer of claim 34 further comprising a light source directed housed within the analyzer housing and directed toward the cartridge.

36. The analyzer of claim 34 further comprising a detector which detects and captures a digital image of fluorescent emissions of the cartridge.

37. The analyzer of claim 36 wherein the detector comprises a charge-coupled device (CCD);
an optical digital camera; a complementary-metal-oxide-semiconductor (CMOS) detector; or a spectrophotometer capable of detecting UV, visible, or infrared wavelengths of light.

38. The analyzer of claim 36 further comprising a processor programmed to analyze the digital image, measuring the intensity of emissions around each bead and correlating measured intensity of the emissions to an amount of target component present in the blood sample material.

39. The analyzer of claim 34 further comprising a display upon which the results of the analysis are displayed.

40. A method of detecting allergen specific IgE comprising:

coating one or more beads with analyte specific capturing ligands, wherein the beads are at least partially contained in one or more wells on a microchip contained in or on a cartridge;

passing a sample to be analyzed for the presence of an analyte over the beads; and

applying an agent which attaches to the bound analyte and enhance detection of a bound analyte.

41. A method of diagnosis of an allergen sensitivity comprising:

obtaining a sample of blood; and

introducing all or part of the blood sample into a receptacle, that is located at least partially in a cartridge and is coupled to a chamber in the cartridge having at least a microchip comprising one or more wells, each well at least partially containing a bead that is coated with an analyte-specific ligand which binds to the analyte contained in the sample as it flows into the chamber from the receptacle.

* * * * *

专利名称(译)	检测人或动物免疫球蛋白-e		
公开(公告)号	US20080176253A1	公开(公告)日	2008-07-24
申请号	US11/746941	申请日	2007-05-10
申请(专利权)人(译)	德州大学系统的校董会		
当前申请(专利权)人(译)	德州大学系统的校董会		
[标]发明人	CHRISTODOULIDES NICOLAOS FLORIANO PIERRE N BALLARD KARRI MCDEVITT JOHN T		
发明人	CHRISTODOULIDES, NICOLAOS FLORIANO, PIERRE N. BALLARD, KARRI MCDEVITT, JOHN T.		
IPC分类号	G01N33/53 C12M1/00		
CPC分类号	G01N33/543 G01N33/6854 G01N33/54366		
优先权	60/799609 2006-05-10 US		
外部链接	Espacenet USPTO		

摘要(译)

描述了用于检测人或动物免疫球蛋白-E的存在的方法，系统和装置。流体或气体样品可以通过盒的基于颗粒的检测系统。可以应用检测和分析技术来确定捕获的IgE的身份和数量。

