



US 20110129818A1

(19) **United States**

(12) **Patent Application Publication**
Adamczyk et al.

(10) **Pub. No.: US 2011/0129818 A1**

(43) **Pub. Date: Jun. 2, 2011**

(54) **ASSAY FOR CARDIAC TROPONIN-T (CTNT)**

Publication Classification

(75) Inventors: **Maciej Adamczyk**, Gurnee, IL (US); **Jeffrey R. Brashear**, Mundelein, IL (US); **Phillip G. Mattingly**, Third Lake, IL (US)

(51) **Int. Cl.**
C12Q 1/68 (2006.01)
G01N 33/53 (2006.01)
(52) **U.S. Cl.** **435/6**; 435/7.1; 435/7.92

(73) Assignee: **ABBOTT LABORATORIES**, Abbott Park, IL (US)

(57) **ABSTRACT**

(21) Appl. No.: **12/629,736**

The present disclosure describes immunoassays for detecting cardiac troponin-T (cTnT) in a test sample, and in particular immunoassays and kits for detecting cTnT in a test sample suspected of containing substances that may interfere with the determination of cTnT, such as heterophilic endogenous antibodies and autoantibodies to cTnT. The methods use more than one capture phase antibody and more than one detection antibody to improve specificity, and provide for the use of humanized immunoreagents to overcome heterophilic antibody interferences.

(22) Filed: **Dec. 2, 2009**

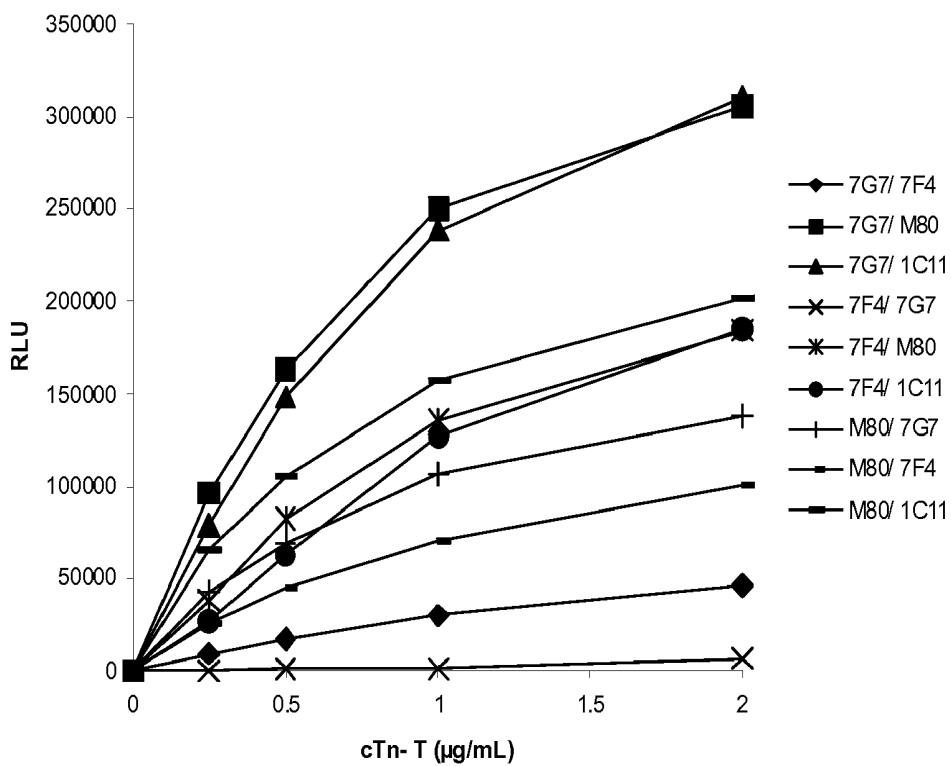


FIG. 1

SDIEEVVEEY.EEEEQEEAAV EEEEDWREDE DEQEEAAEED AEAEAETEET
RAEEDEEEE AKEAEDGPME ESKPKPRSFM PNLVPPKIPD GERVDFDDIH
RKRMEKDLNE LQALIEAHFE NRKKEEELV SLKDRIERRR AERAEQQRIR
NEREKERQNR LAERARREE EENRRKAEDE ARKKKALSNM MHFGGYIQKQ
AQTERKSGKR QTEREKKKKI LAERRKVLAI DHLNEDQLRE KAKELWQSIY
NLEAEKFDLQ EKFKQKYEI NVLRNRINDN QKVS KTRGKA KVTGRWK

(297 aa)

FIG. 2

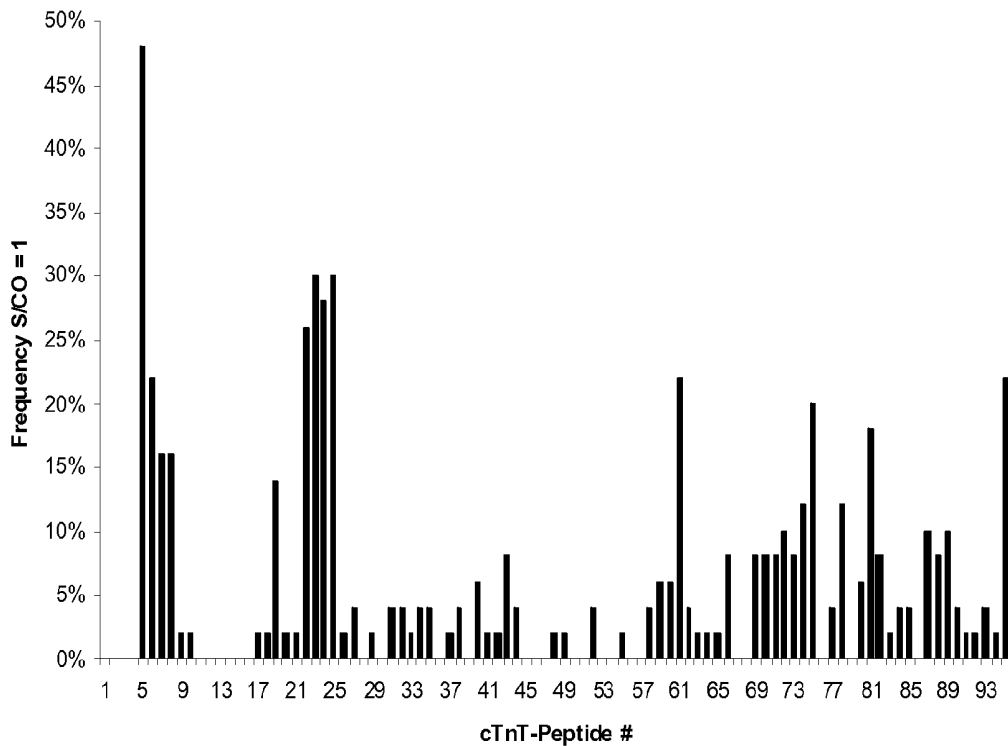


FIG. 3

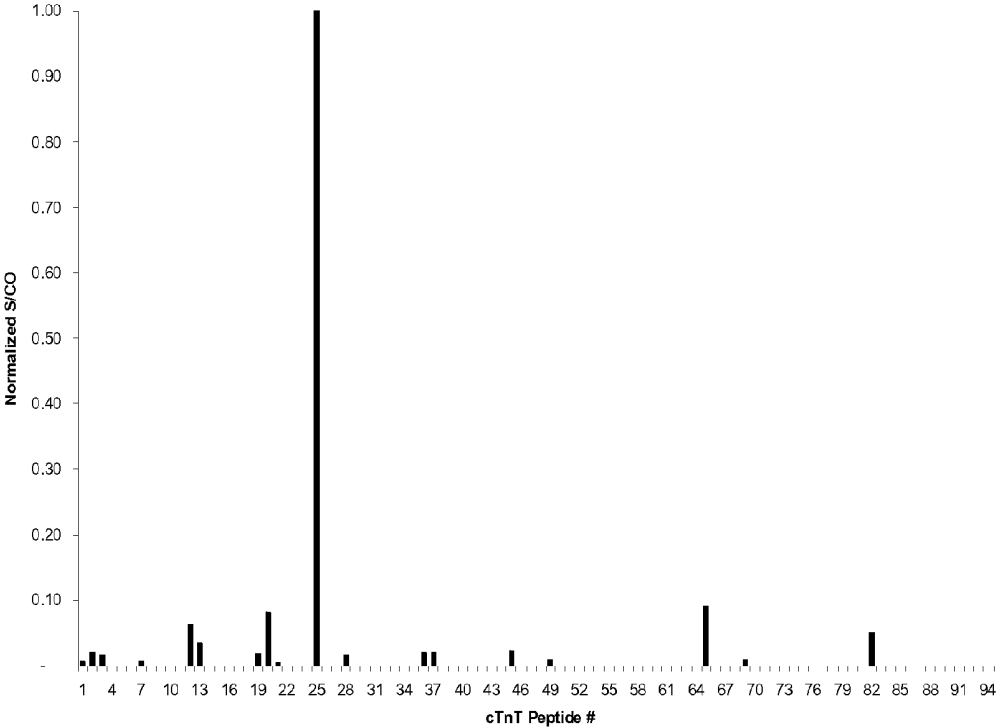


FIG. 4

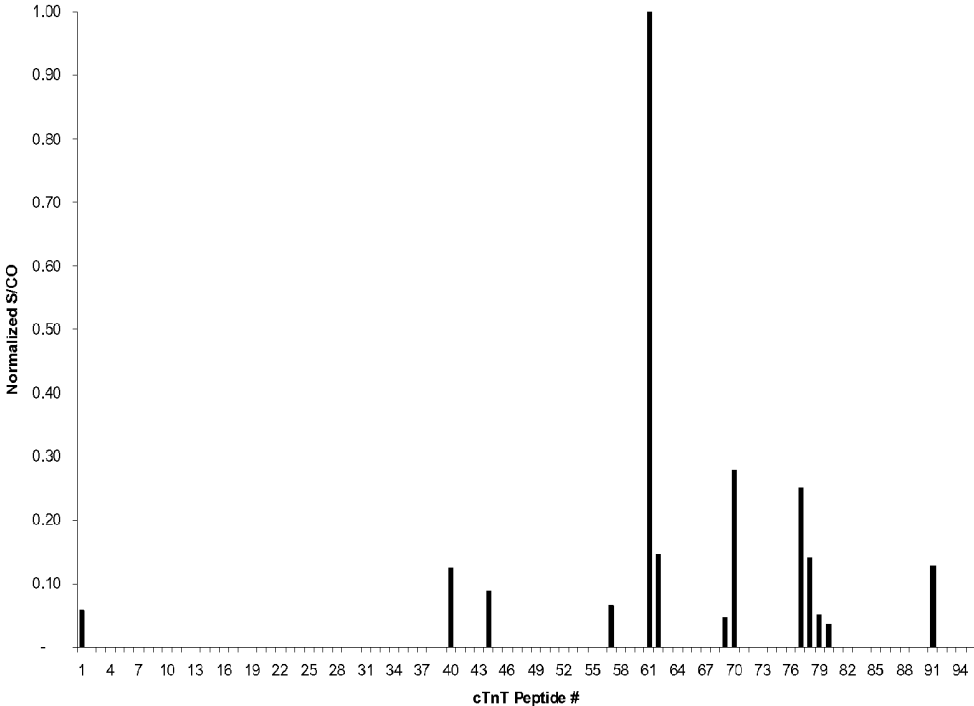


FIG. 5

ASSAY FOR CARDIAC TROPONIN-T (CTNT)

RELATED APPLICATION INFORMATION

[0001] None.

TECHNICAL FIELD

[0002] The present disclosure relates generally to assays and kits for detecting cardiac troponin-T (cTnT) in a test sample, and in particular to methods and kits for detecting cTnT in a test sample suspected of containing substances that may interfere with the determination of cTnT.

BACKGROUND OF THE INVENTION

[0003] Immunoassay techniques have been known for the last few decades and are now commonly used in medicine for a wide variety of diagnostic purposes to detect target analytes in a biological sample. Immunoassays exploit the highly specific binding of an antibody to its corresponding antigen, wherein the antigen is the target analyte. Typically, quantification of either the antibody or antigen is achieved through some form of labeling such as radio- or fluorescence-labeling. Sandwich immunoassays involve binding the target analyte in the sample to the antibody site (which is frequently bound to a solid support), binding labeled antibody to the captured analyte, and then measuring the amount of bound labeled antibody, wherein the label generates a signal proportional to the concentration of the target analyte inasmuch as labeled antibody does not bind unless the analyte is present in the sample.

[0004] Cardiac troponins are sensitive and specific biomarkers of cardiac injury. In particular, cTnT is highly cardiac specific, and it is not present in serum following non-myocardial muscle or other tissue damage. In addition, cTnT has been shown to be a more persistent and sensitive biomarker than others used for diagnosing myocardial infarction. Thus cardiac troponins generally are generally useful for diagnosing acute myocardial ischemia, and cTnT is especially useful. Currently a single assay is available for cTnT detection, from Roche Diagnostics. The assay is reportedly limited to detecting human cTnT from human heart tissue to only 7%. (C. Cobbaert et al, *Mv. Ned Tijdschr KIM Chem Labgeneesk* 2007; 32:175-8). Additionally, like many others, assays for cTnT are subject to interference heterophilic endogenous antibodies, which produce false positive results and thus misdiagnosis (G. H. White et al., *Clin Chem* 2002; 48:201-3; N. Shayanfar et al., *Swiss Med Wkly* 2008; 138:470). False negatives have also been reported. (See, e.g., Mahalingam M, Ottlinger M E. False-negative qualitative cardiac troponin in a 79-year-old man with myocardial infarction. *JAMA* 1997; 278:2143-4.J).

[0005] Additionally, the known assay for cTnT fails to address the problem of circulating endogenous antibodies, or "autoantibodies". Autoantibodies have been described for cTnT in apparently healthy blood donors (Adamczyk, M., Brashear, R. J., and Mattingly, P. G. (2009) *Clin Chem* 55, 1592-3; see also US Patent Application No. US20080102481A1). Other previously described autoantibodies are known to create interference in typical sandwich immunoassays composed of two or more analyte-specific antibodies. For example, cardiac troponin-I reactive autoantibodies may interfere with the measurement of cTnI using conventional midfragment-specific immunoassays. Thus, interference from autoantibodies can also produce erroneous

results, particularly near the cut-off values established for clinical diagnoses, thereby increasing the risk of false negative diagnostic results and the risk that individuals will not obtain a timely diagnosis. Additionally, autoantibodies may react with antigens, forming macro-complexes which may extend the circulating half-life of the antigen beyond the typical course of the acute release of the antigen. One approach to addressing the problem of interference from autoantibodies is to choose analyte-specific antibodies that bind to specific epitopes distinct from the analyte epitopes that react with the autoantibodies. Following this general approach, efforts have focused on exploring the use of thousands of different combinations of two, three and even four analyte-specific antibodies to avoid interference from autoantibodies. However, this effort has been largely unsuccessful. It is now evident that autoantibodies against complex protein analytes are likely to be polyclonal within a particular sample, and may be even more diverse among samples from different individuals. Interference from diverse polyclonal autoantibodies may explain the observation that as little as 25% or even less of an analyte protein sequence binds to analyte-specific antibodies, which may in turn explain the lack of success using this approach.

[0006] A need therefore exists in the art for improved cTnT immunoassay methods that compensate for interference from various substances that may also be present in a test sample, and in particular for such methods that do so without involving redesign of the analyte detection or capture antibodies.

SUMMARY OF THE INVENTION

[0007] In one aspect, the present disclosure provides an immunoassay for quantifying an amount of cardiac troponin-T (cTnT) in a test sample, the immunoassay comprising the steps of:

[0008] a) contacting a test sample suspected of containing cTnT with n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody: cTnT complex $(C_1)(C_2) \dots (C_n)(cTnT)$, wherein n is an integer from 1 to 10; and

[0009] b) contacting said mixture comprising a n-capture antibody-cTnT epitope complex $(C_1)(C_2) \dots (C_n)(cTnT)$ with n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody: n-capture antibody: cTnT measurable assembly $(D_1)(D_2) \dots (D_{n'}) (C_1)(C_2) \dots (C_n)(cTnT)$, wherein n' and n are independently an integer from 1 to 10, and antibodies C and D bind to (n+n') different epitopes of cTnT.

[0010] In the immunoassay, an optical, electrical, or change-of-state signal of the measurable assembly can be measured. An optical signal may be measured as a cTnT concentration dependent change in chemiluminescence, fluorescence, phosphorescence, electrochemiluminescence, ultraviolet absorption, visible absorption, infrared absorption, refraction, surface plasmon resonance. An electrical signal may be measured as a cTnT dependent change in current, resistance, potential, mass to charge ratio, or ion count. Alternatively, the change-of-state signal may be measured as a cTnT concentration dependent change in size, solubility, mass, or resonance.

[0011] In the above immunoassay, the capture antibodies, the detection antibodies, or the capture and detection antibodies may comprise humanized antibodies.

[0012] In the above immunoassay, the detection antibodies can be conjugated to a detectable label, wherein the detectable label is an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

[0013] In the above immunoassay, detection antibodies may comprise humanized antibodies complexed with an anti-human IgG antibody, which may be conjugated to a detectable label. The detectable label is for example an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

[0014] In the above immunoassay, the capture antibodies may be immobilized on a solid phase. The solid phase may be selected from the group consisting of a magnetic particle, bead, test tube, microtiter plate, cuvette, membrane, a scaffolding molecule, quartz crystal, film, filter paper, disc and chip.

[0015] In another aspect, the present disclosure provides an immunoassay for quantifying an amount of cTnT in a test sample, the immunoassay comprising the steps of:

[0016] a) contacting a test sample suspected of containing cTnT with n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody:cTnT complex (C₁)(C₂) . . . (C_n)(cTnT), wherein n is an integer from 1 to 10;

[0017] b) contacting said mixture comprising a n-capture antibody-cTnT epitope complex (C₁)(C₂) . . . (C_n)(cTnT) with n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody:n-capture antibody:cTnT measurable assembly (D₁)(D₂) . . . (D_{n'})(C₁)(C₂) . . . (C_n)(cTnT), wherein the detection antibodies D are labeled with a detectable label comprising at least one acridinium compound, n' and n are independently an integer from 1 to 10, and antibodies C and D bind to (n+n') different epitopes of cTnT;

[0018] c) generating or providing a source of hydrogen peroxide to the mixture of step (b);

[0019] d) adding a basic solution to the mixture of step (c) to generate a light signal;


[0020] e) measuring the light signal generated by or emitted in step (d); and

[0021] f) quantifying the amount of troponin-T in the test sample based on the measurement in step (e).

[0022] In the above immunoassay, the capture antibodies, the detection antibodies, or the capture and detection antibodies may comprise humanized antibodies.

[0023] In the above immunoassay, the detection antibodies may comprise humanized antibodies complexed with an anti-human IgG antibody conjugated to the detectable label that comprises at least one acridinium compound.

[0024] In the above immunoassay, any acridinium compound can be used. For example, the acridinium compound can be an acridinium-9-carboxamide having a structure according to formula I:

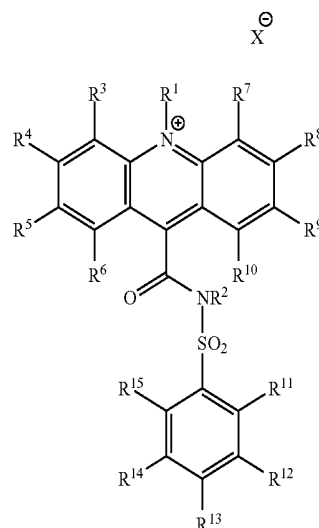


[0025] wherein R¹ and R² are each independently selected from the group consisting of: alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0026] wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0027] optionally, if present, X[⊖] is an anion.

[0028] Alternatively, the acridinium compound is an acridinium-9-carboxylate aryl ester having a structure according to formula II:

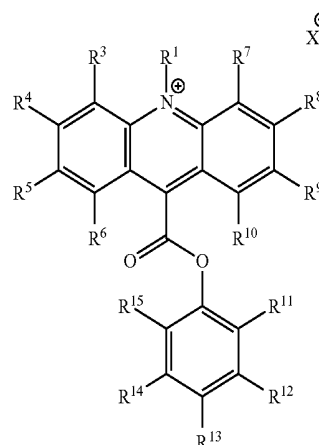

[0029] wherein R¹ is an alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0030] wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0031] optionally, if present, X[⊖] is an anion.

[0032] In the above immunoassay, the capture antibodies C may be immobilized on a solid phase. The solid phase may be selected from the group consisting of a magnetic particle, bead, test tube, microtiter plate, cuvette, membrane, a scaffolding molecule, quartz crystal, film, filter paper, disc and chip.

[0033] In the above immunoassay, the capture antibodies can be selected from the group consisting of a polyclonal antibody, a monoclonal antibody, a chimeric antibody, a human antibody, and an affinity matured antibody. Additionally, the detection antibodies can be selected from the group consisting of a polyclonal antibody, a monoclonal antibody, a chimeric antibody, a human antibody, and an affinity matured antibody.

[0034] In the above immunoassay, the hydrogen peroxide can be provided by adding a buffer or a solution containing hydrogen peroxide. The hydrogen peroxide can be generated by adding a hydrogen peroxide generating enzyme to the test sample. The hydrogen peroxide generating enzyme can be selected from the group consisting of: (R)-6-hydroxynicotine oxidase, (S)-2-hydroxy acid oxidase, (S)-6-hydroxynicotine oxidase, 3-aci-nitropropanoate oxidase, 3-hydroxyanthranilate oxidase, 4-hydroxymandelate oxidase, 6-hydroxynicotinate dehydrogenase, abscisic-aldehyde oxidase, acyl-CoA oxidase, alcohol oxidase, aldehyde oxidase, amine oxidase, amine oxidase (copper-containing), amine oxidase (flavin-containing), aryl-alcohol oxidase, aryl-aldehyde oxidase, catechol oxidase, cholesterol oxidase, choline oxidase, columbamine oxidase, cyclohexylamine oxidase, cytochrome c oxidase, D-amino-acid oxidase, D-arabinono-1,4-lactone oxidase, D-arabinono-1,4-lactone oxidase, D-aspartate oxidase, D-glutamate oxidase, D-glutamate(D-aspartate) oxidase, dihydrobenzophenanthridine oxidase, dihydroorotate oxidase, dihydrouracil oxidase, dimethylglycine oxidase, D-mannitol oxidase, ecdysone oxidase, ethanolamine oxidase, galactose oxidase, glucose oxidase, glutathione oxidase, glycerol-3-phosphate oxidase, glycine oxidase, glyoxylate oxidase, hexose oxidase, hydroxyphytanate oxidase, indole-3-acetaldehyde oxidase, lactic acid oxidase, L-amino-acid oxidase, L-aspartate oxidase, L-galactonolactone oxidase, L-glutamate oxidase, L-gulonolactone oxidase, L-lysine 6-oxidase, L-lysine oxidase, long-chain-alcohol oxidase, L-pipecolate oxidase, L-sorbose oxidase, malate oxidase, methanethiol oxidase, monoamino acid oxidase, N6-methyl-lysine oxidase, N-acylhexosamine oxidase, NAD (P)H oxidase, nitroalkane oxidase, N-methyl-L-amino-acid oxidase, nucleoside oxidase, oxalate oxidase, polyamine oxidase, polyphenol oxidase, polyvinyl-alcohol oxidase, prenyl-cysteine oxidase, protein-lysine 6-oxidase, putrescine oxidase, pyranose oxidase, pyridoxal 5'-phosphate synthase, pyridoxine 4-oxidase, pyrroloquinoline-quinone synthase, pyruvate oxidase, pyruvate oxidase (CoA-acetylating), reticuline oxidase, retinal oxidase, rifamycin-B oxidase, sarcosine oxidase, secondary-alcohol oxidase, sulfite oxidase, superoxide dismutase, superoxide reductase, tetrahydroberberine oxidase, thiamine oxidase, tryptophan α,β -oxidase, urate oxidase (uricase, uric acid oxidase), vanillyl-alcohol oxidase, xanthine oxidase, xylitol oxidase and combinations thereof.

[0035] In the above immunoassay, the basic solution can be for example a solution having a pH of at least about 10.

[0036] The above immunoassay may further comprise the step of quantifying the amount of the cTnT in the test sample by relating the amount of light signal in step (e) to the amount

of cTnT in the test sample either by use of a standard curve for cTnT or by comparison to a reference standard. The reference standard may comprise an anti-idiotypic antibody. The reference standard may comprise a derivatized cTnT, such as for example cTnT derivatized with a polyethylene glycol.

[0037] The above immunoassay may be adapted for use in an automated system or semi-automated system.

[0038] In any of the above immunoassays, the test sample may be whole blood, serum, or plasma.

[0039] In another aspect, the present disclosure provides a kit for quantifying the amount of cTnT in a test sample, the kit comprising:

[0040] a) n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody: cTnT complex $(C_1)(C_2) \dots (C_n)(cTnT)$, wherein n is an integer from 1 to 10;

[0041] b) n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody:n-capture antibody: cTnT measurable assembly $(D_1)(D_2) \dots (D_{n'}) (C_1)(C_2) \dots (C_n)(cTnT)$, wherein n' and n are independently an integer from 1 to 10; and wherein antibodies C and D bind to (n+n') different epitopes of cTnT; and

[0042] c) instructions for quantifying the amount of troponin-T in the test sample.


[0043] In the above kit, the capture antibodies, the detection antibodies, or the capture and detection antibodies may comprise humanized antibodies.

[0044] In the above kit, the detection antibodies may comprise humanized antibodies complexed to an antihuman IgG antibody. The antihuman IgG antibody may be conjugated to the detectable label.

[0045] In the above kit, the capture antibodies may be bound to a solid phase. The solid phase can be selected from the group consisting of a magnetic particle, a bead, a test tube, a microtiter plate, a cuvette, a membrane, a scaffolding molecule, a quartz crystal, a film, a filter paper, a disc and a chip.

[0046] The above kit may further comprise a detectable label conjugated to the detection antibodies. The detectable label may be an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

[0047] In the above kit, an acridinium compound can be used as the detectable label. For example, the acridinium compound can be an acridinium-9-carboxamide having a structure according to formula I:

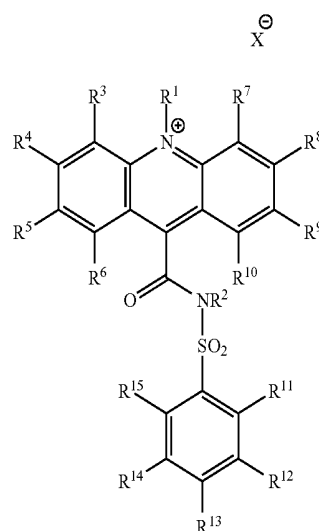


I

[0048] wherein R¹ and R² are each independently selected from the group consisting of: alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl, and wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0049] optionally, if present, X[⊖] is an anion.

[0050] Alternatively, in the above kit the acridinium compound is an acridinium-9-carboxylate aryl ester having a structure according to formula II:

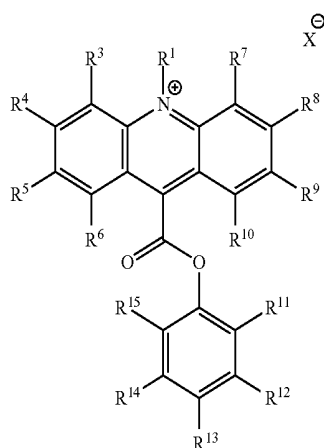

[0051] wherein R¹ is an alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0052] wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0053] optionally, if present, X[⊖] is an anion.

[0054] The above kit may further comprise a basic solution. The basic solution can be for example a solution having a pH of at least about 10.

[0055] The above kit may further include a hydrogen peroxide source, which can be a buffer, a solution containing hydrogen peroxide, or a hydrogen peroxide generating enzyme. In kits containing a hydrogen peroxide generating enzyme, the enzyme can be selected from the group consisting of: (R)-6-hydroxynicotine oxidase, (S)-2-hydroxy acid oxidase, (S)-6-hydroxynicotine oxidase, 3-aci-nitropropanoate oxidase, 3-hydroxyanthranilate oxidase, 4-hydroxymandelate oxidase, 6-hydroxynicotinate dehydrogenase, abscisic-aldehyde oxidase, acyl-CoA oxidase, alcohol oxidase, aldehyde oxidase, amine oxidase, amine oxidase (copper-containing), amine oxidase (flavin-containing), aryl-alcohol oxidase, aryl-aldehyde oxidase, catechol oxidase, cholesterol oxidase, choline oxidase, columbamine oxidase, cyclohexylamine oxidase, cytochrome c oxidase, D-amino acid oxidase, D-arabinono-1,4-lactone oxidase, D-arabinono-1,4-lactone oxidase, D-aspartate oxidase, D-glutamate oxidase, D-glutamate(D-aspartate) oxidase, dihydrobenzophenanthridine oxidase, dihydroorotate oxidase, dihydrouracil oxidase, dimethylglycine oxidase, D-mannitol oxidase, ecdysone oxidase, ethanolamine oxi-

dase, galactose oxidase, glucose oxidase, glutathione oxidase, glycerol-3-phosphate oxidase, glycine oxidase, glyoxylate oxidase, hexose oxidase, hydroxyphytanate oxidase, indole-3-acetaldehyde oxidase, lactic acid oxidase, L-amino acid oxidase, L-aspartate oxidase, L-galactonolactone oxidase, L-glutamate oxidase, L-gulonolactone oxidase, L-lysine 6-oxidase, L-lysine oxidase, long-chain-alcohol oxidase, L-pipecolate oxidase, L-sorbose oxidase, malate oxidase, methanethiol oxidase, monoamino acid oxidase, N6-methyl-lysine oxidase, N-acylhexosamine oxidase, NAD (P)H oxidase, nitroalkane oxidase, N-methyl-L-amino acid oxidase, nucleoside oxidase, oxalate oxidase, polyamine oxidase, polyphenol oxidase, polyvinyl-alcohol oxidase, prenyl-cysteine oxidase, protein-lysine 6-oxidase, putrescine oxidase, pyranose oxidase, pyridoxal 5'-phosphate synthase, pyridoxine 4-oxidase, pyrroloquinoline-quinone synthase, pyruvate oxidase, pyruvate oxidase (CoA-acetylating), reticuline oxidase, retinal oxidase, rifamycin-B oxidase, sarcosine oxidase, secondary-alcohol oxidase, sulfite oxidase, superoxide dismutase, superoxide reductase, tetrahydroberberine oxidase, thiamine oxidase, tryptophan α,β -oxidase, urate oxidase (uricase, uric acid oxidase), vanillyl-alcohol oxidase, xanthine oxidase, xylitol oxidase and combinations thereof.

[0056] The above kit may further comprise a cTnT reference standard. The cTnT reference standard may comprise, for example, an anti-idiotypic antibody. The cTnT reference standard may comprise a derivatized cTnT, such as for example cTnT derivatized with a polyethylene glycol.

BRIEF DESCRIPTION OF THE DRAWINGS

[0057] FIG. 1 is a graph of dose-response of different combinations of detection and capture antibodies;

[0058] FIG. 2 is the amino acid sequence of Human cardiac troponin T (cTnT);

[0059] FIG. 3 is a frequency plot of cTnT autoantibody epitopes;

[0060] FIG. 4 is an epitope map of murine anti-cardiac troponin-T M8020207; and

[0061] FIG. 5 is an epitope map of murine anti-cardiac troponin-T 1C11.

DETAILED DESCRIPTION

[0062] The present disclosure provides an improved assay for quantifying an amount of cTnT in a test sample, and especially in a test sample suspected of containing substances that may interfere with the determination of cTnT in the sample. Such substances include but are not limited to, for example, endogenous anti-cTnT antibodies. The methods are based in part on the use of more than one capture phase antibody and more than one detection antibody to improve specificity. This assay approach compensates for the presence of other substances such as heterophilic endogenous antibodies, and autoantibodies that may be present in the test sample without redesign of the analyte-specific detection antibodies or the capture antibodies, and avoids the need of a second assay to identify problematic samples.

[0063] Additionally, the methods provide for the use of humanized immunoreagents to overcome heterophilic antibody interferences. Use of antihuman IgG detection antibody corrects for endogenous autoantibodies and when used in conjunction with humanized immunoreagents provides a

“universal” signal generator. Derivatized cTnT provides a soluble reagent suitable for assay standardization.

A. DEFINITIONS

[0064] Section headings as used in this section and the entire disclosure herein are not intended to be limiting.

[0065] As used herein, the singular forms “a,” “an” and “the” include plural referents unless the context clearly dictates otherwise. For the recitation of numeric ranges herein, each intervening number there between with the same degree of precision is explicitly contemplated. For example, for the range 6-9, the numbers 7 and 8 are contemplated in addition to 6 and 9, and for the range 6.0-7.0, the numbers 6.0, 6.1, 6.2, 6.3, 6.4, 6.5, 6.6, 6.7, 6.8, 6.9 and 7.0 are explicitly contemplated.

[0066] a) Acyl (and Other Chemical Structural Group Definitions)

[0067] As used herein, the term “acyl” refers to a $-\text{C}(\text{O})\text{R}_a$ group where R_a is hydrogen, alkyl, cycloalkyl, cycloalkylalkyl, phenyl or phenylalkyl. Representative examples of acyl include, but are not limited to, formyl, acetyl, cyclohexylcarbonyl, cyclohexylmethylcarbonyl, benzoyl, benzylcarbonyl and the like.

[0068] As used herein, the term “alkenyl” means a straight or branched chain hydrocarbon containing from 2 to 10 carbons and containing at least one carbon-carbon double bond formed by the removal of two hydrogens. Representative examples of alkenyl include, but are not limited to, ethenyl, 2-propenyl, 2-methyl-2-propenyl, 3-butenyl, 4-pentenyl, 5-hexenyl, 2-heptenyl, 2-methyl-1-heptenyl, and 3-decenyl.

[0069] As used herein, the term “alkyl” means a straight or branched chain hydrocarbon containing from 1 to 10 carbon atoms. Representative examples of alkyl include, but are not limited to, methyl, ethyl, n-propyl, iso-propyl, n-butyl, sec-butyl, iso-butyl, tert-butyl, n-pentyl, isopentyl, neopentyl, n-hexyl, 3-methylhexyl, 2,2-dimethylpentyl, 2,3-dimethylpentyl, n-heptyl, n-octyl, n-nonyl, and n-decyl.

[0070] As used herein, the term “alkyl radical” means any of a series of univalent groups of the general formula $\text{C}_n\text{H}_{2n+1}$ derived from straight or branched chain hydrocarbons.

[0071] As used herein, the term “alkoxy” means an alkyl group, as defined herein, appended to the parent molecular moiety through an oxygen atom. Representative examples of alkoxy include, but are not limited to, methoxy, ethoxy, propoxy, 2-propoxy, butoxy, tert-butoxy, pentyloxy, and hexyloxy.

[0072] As used herein, the term “alkynyl” means a straight or branched chain hydrocarbon group containing from 2 to 10 carbon atoms and containing at least one carbon-carbon triple bond. Representative examples of alkynyl include, but are not limited, to acetylenyl, 1-propynyl, 2-propynyl, 3-butynyl, 2-pentynyl, and 1-butynyl.

[0073] As used herein, the term “amido” refers to an amino group attached to the parent molecular moiety through a carbonyl group (wherein the term “carbonyl group” refers to a $-\text{C}(\text{O})-$ group).

[0074] As used herein, the term “amino” means $-\text{NR}_b\text{R}_c$, wherein R_b and R_c are independently selected from the group consisting of hydrogen, alkyl and alkylcarbonyl.

[0075] As used herein, the term “arylalkyl” means an aryl group appended to the parent molecular moiety through an alkyl group, as defined herein. Representative examples of arylalkyl include, but are not limited to, benzyl, 2-phenylethyl, 3-phenylpropyl, and 2-naphth-2-ylethyl.

[0076] As used herein, the term “aryl” means a phenyl group, or a bicyclic or tricyclic fused ring system wherein one or more of the fused rings is a phenyl group. Bicyclic fused ring systems are exemplified by a phenyl group fused to a cycloalkenyl group, a cycloalkyl group, or another phenyl group. Tricyclic fused ring systems are exemplified by a bicyclic fused ring system fused to a cycloalkenyl group, a cycloalkyl group, as defined herein or another phenyl group. Representative examples of aryl include, but are not limited to, anthracenyl, azulenyl, fluorenyl, indanyl, indenyl, naphthyl, phenyl, and tetrahydronaphthyl. The aryl groups of the present disclosure can be optionally substituted with one-, two, three, four, or five substituents independently selected from the group consisting of alkoxy, alkyl, carboxyl, halo, and hydroxyl.

[0077] As used herein, the term “carboxy” or “carboxyl” refers to $-\text{CO}_2\text{H}$ or $-\text{CO}_2^-$.

[0078] As used herein, the term “carboxyalkyl” refers to a $-(\text{CH}_2)_n\text{CO}_2\text{H}$ or $-(\text{CH}_2)_n\text{CO}_2^-$ group where n is from 1 to 10.

[0079] As used herein, the term “cyano” means a $-\text{CN}$ group.

[0080] As used herein, the term “cycloalkenyl” refers to a non-aromatic cyclic or bicyclic ring system having from three to ten carbon atoms and one to three rings, wherein each five-membered ring has one double bond, each six-membered ring has one or two double bonds, each seven- and eight-membered ring has one to three double bonds, and each nine- to ten-membered ring has one to four double bonds. Representative examples of cycloalkenyl groups include cyclohexenyl, octahydronaphthalenyl, norbornenyl, and the like. The cycloalkenyl groups can be optionally substituted with one, two, three, four, or five substituents independently selected from the group consisting of alkoxy, alkyl, carboxyl, halo, and hydroxyl.

[0081] As used herein, the term “cycloalkyl” refers to a saturated monocyclic, bicyclic, or tricyclic hydrocarbon ring system having three to twelve carbon atoms. Representative examples of cycloalkyl groups include cyclopropyl, cyclopentyl, bicyclo[3.1.1]heptyl, adamantyl, and the like. The cycloalkyl groups of the present disclosure can be optionally substituted with one, two, three, four, or five substituents independently selected from the group consisting of alkoxy, alkyl, carboxyl, halo, and hydroxyl.

[0082] As used herein, the term “cycloalkylalkyl” means a $-\text{R}_d\text{R}_e$ group where R_d is an alkylene group and R_e is cycloalkyl group. A representative example of a cycloalkylalkyl group is cyclohexylmethyl and the like.

[0083] As used herein, the term “halogen” means a $-\text{Cl}$, $-\text{Br}$, $-\text{I}$ or $-\text{F}$; the term “halide” means a binary compound, of which one part is a halogen atom and the other part is an element or radical that is less electronegative than the halogen, e.g., an alkyl radical.

[0084] As used herein, the term “hydroxyl” means an $-\text{OH}$ group.

[0085] As used herein, the term “nitro” means a $-\text{NO}_2$ group.

[0086] As used herein, the term “oxoalkyl” refers to $-(\text{CH}_2)_n\text{C}(\text{O})\text{R}_a$, where R_a is hydrogen, alkyl, cycloalkyl, cycloalkylalkyl, phenyl or phenylalkyl and where n is from 1 to 10.

[0087] As used herein, the term “phenylalkyl” means an alkyl group which is substituted by a phenyl group.

[0088] As used herein, the term “sulfo” means a $-\text{SO}_3\text{H}$ group.

[0089] As used herein, the term “sulfoalkyl” refers to a $-(\text{CH}_2)_n-\text{SO}_3\text{H}$ or $-(\text{CH}_2)_n-\text{SO}_3^-$ group where n is from 1 to 10.

[0090] b) Anion

[0091] As used herein, the term “anion” refers to an anion of an inorganic or organic acid, such as, but not limited to, hydrochloric acid, hydrobromic acid, sulfuric acid, methanesulfonic acid, formic acid, acetic acid, oxalic acid, succinic acid, tartaric acid, mandelic acid, fumaric acid, lactic acid, citric acid, glutamic acid, aspartic acid, phosphate, trifluoromethanesulfonic acid, trifluoroacetic acid and fluorosulfonic acid and any combinations thereof.

[0092] c) Antibody

[0093] As used herein, the term “antibody” refers to a protein consisting of one or more polypeptides substantially

encoded by immunoglobulin genes or fragments of immunoglobulin genes, and encompasses polyclonal antibodies, monoclonal antibodies, and fragments thereof, as well as molecules engineered from immunoglobulin gene sequences. The recognized immunoglobulin genes include the kappa, lambda, alpha, gamma, delta, epsilon and mu constant region genes, as well as myriad immunoglobulin variable region genes. Light chains are classified as either kappa or lambda. Heavy chains are classified as gamma, mu, alpha, delta, or epsilon, which in turn define the immunoglobulin classes, IgG, IgM, IgA, IgD and IgE, respectively.

[0094] d) Hydrogen Peroxide Generating Enzyme

[0095] As used herein, the term “hydrogen peroxide generating enzyme” refers to an enzyme that is capable of producing as a reaction product the chemical compound having the molecular formula H_2O_2 , i.e. hydrogen peroxide. Non-limiting examples of hydrogen peroxide generating enzymes are listed below in Table 1.

TABLE 1

ACCEPTED COMMON NAME	IUBMB ENZYME NOMENCLATURE	PREFERRED SUBSTRATE
(R)-6-hydroxynicotine oxidase	EC 1.5.3.6	(R)-6-hydroxynicotine
(S)-2-hydroxy acid oxidase	EC 1.1.3.15	S)-2-hydroxy acid
(S)-6-hydroxynicotine oxidase	EC 1.5.3.5	(S)-6-hydroxynicotine
3-aci-nitropropanoate oxidase	EC 1.7.3.5	3-aci-nitropropanoate
3-hydroxyanthranilate oxidase	EC 1.10.3.5	3-hydroxyanthranilate
4-hydroxymandelate oxidase	EC 1.1.3.19	(S)-2-hydroxy-2-(4-hydroxyphenyl)acetate
6-hydroxynicotinate dehydrogenase	EC 1.17.3.3	6-hydroxynicotinate
Abscisic-aldehyde oxidase	EC 1.2.3.14	abscisic aldehyde
acyl-CoA oxidase	EC 1.3.3.6	acyl-CoA
Alcohol oxidase	EC 1.1.3.13	a primary alcohol
Aldehyde oxidase	EC 1.2.3.1	an aldehyde
amine oxidase		
amine oxidase (copper-containing)	EC 1.4.3.6	primary monoamines, diamines and histamine
amine oxidase (flavin-containing)	EC 1.4.3.4	a primary amine
aryl-alcohol oxidase	EC 1.1.3.7	an aromatic primary alcohol (2-naphthyl)methanol 3-methoxybenzyl alcohol an aromatic aldehyde
aryl-aldehyde oxidase	EC 1.2.3.9	
Catechol oxidase	EC 1.1.3.14	Catechol
cholesterol oxidase	EC 1.1.3.6	Cholesterol
Choline oxidase	EC 1.1.3.17	Choline
columbamine oxidase	EC 1.21.3.2	Columbamine
cyclohexylamine oxidase	EC 1.4.3.12	Cyclohexylamine
cytochrome c oxidase	EC 1.9.3.1	
D-amino-acid oxidase	EC 1.4.3.3	a D-amino acid
D-arabinono-1,4-lactone oxidase	EC 1.1.3.37	D-arabinono-1,4-lactone
D-arabinono-1,4-lactone oxidase	EC 1.1.3.37	D-arabinono-1,4-lactone
D-aspartate oxidase	EC 1.4.3.1	D-aspartate
D-glutamate oxidase	EC 1.4.3.7	D-glutamate
D-glutamate(D-aspartate) oxidase	EC 1.4.3.15	D-glutamate
dihydrobenzophenanthridine oxidase	EC 1.5.3.12	dihydrosanguinarine
dihydroorotate oxidase	EC 1.3.3.1	(S)-dihydroorotate
dihydrouracil oxidase	EC 1.3.3.7	5,6-dihydrouracil
dimethylglycine oxidase	EC 1.5.3.10	N,N-dimethylglycine
D-mannitol oxidase	EC 1.1.3.40	Mannitol
Ecdysone oxidase	EC 1.1.3.16	Ecdysone
ethanolamine oxidase	EC 1.4.3.8	Ethanolamine
Galactose oxidase	EC 1.1.3.9	D-galactose
Glucose oxidase	EC 1.1.3.4	β -D-glucose
glutathione oxidase	EC 1.8.3.3	Glutathione
Glycerol-3-phosphate oxidase	EC 1.1.3.21	sn-glycerol 3-phosphate
Glycine oxidase	EC 1.4.3.19	Glycine
glyoxylate oxidase	EC 1.2.3.5	Glyoxylate
hexose oxidase	EC 1.1.3.5	D-glucose, D-galactose D-mannose maltose lactose cellobiose

TABLE 1-continued

ACCEPTED COMMON NAME	IUBMB ENZYME NOMENCLATURE	PREFERRED SUBSTRATE
hydroxyphytanate oxidase	EC 1.1.3.27	L-2-hydroxyphytanate
indole-3-acetaldehyde oxidase	EC 1.2.3.7	(indol-3-yl)acetaldehyde
lactic acid oxidase		Lactic acid
L-amino-acid oxidase	EC 1.4.3.2	an L-amino acid
L-aspartate oxidase	EC 1.4.3.16	L-aspartate
L-galactonolactone oxidase	EC 1.3.3.12	L-galactono-1,4-lactone
L-glutamate oxidase	EC 1.4.3.11	L-glutamate
L-gulonolactone oxidase	EC 1.1.3.8	L-gulono-1,4-lactone
L-lysine 6-oxidase	EC 1.4.3.20	L-lysine
L-lysine oxidase	EC 1.4.3.14	L-lysine
long-chain-alcohol oxidase	EC 1.1.3.20	A long-chain-alcohol
L-pipecolate oxidase	EC 1.5.3.7	L-pipecolate
L-sorbose oxidase	EC 1.1.3.11	L-sorbose
malate oxidase	EC 1.1.3.3	(S)-malate
methanethiol oxidase	EC 1.8.3.4	Methanethiol
monoamino acid oxidase		
N ⁶ -methyl-lysine oxidase	EC 1.5.3.4	6-N-methyl-L-lysine
N-acylhexosamine oxidase	EC 1.1.3.29	N-acetyl-D-glucosamine N-glycolylglucosamine N-acetylgalactosamine N-acetylmannosamine.
NAD(P)H oxidase	EC 1.6.3.1	NAD(P)H
nitroalkane oxidase	EC 1.7.3.1	a nitroalkane
N-methyl-L-amino-acid oxidase	EC 1.5.3.2	an N-methyl-L-amino acid
nucleoside oxidase	EC 1.1.3.39	Adenosine
Oxalate oxidase	EC 1.2.3.4	Oxalate
polyamine oxidase	EC 1.5.3.11	1-N-acetylspermine
polyphenol oxidase	EC 1.14.18.1	
Polyvinyl-alcohol oxidase	EC 1.1.3.30	polyvinyl alcohol
prenylcysteine oxidase	EC 1.8.3.5	an S-prenyl-L-cysteine
Protein-lysine 6-oxidase	EC 1.4.3.13	peptidyl-L-lysyl-peptide
putrescine oxidase	EC 1.4.3.10	butane-1,4-diamine
Pyranose oxidase	EC 1.1.3.10	D-glucose D-xylose L-sorbose D-glucono-1,5-lactone
Pyridoxal 5'-phosphate synthase	EC 1.4.3.5	pyridoxamine 5'-phosphate
pyridoxine 4-oxidase	EC 1.1.3.12	Pyridoxine
pyrroloquinoline-quinone synthase	EC 1.3.3.11	6-(2-amino-2-carboxyethyl)-7,8-dioxo-1,2,3,4,5,6,7,8-octahydroquinoline-2,4-dicarboxylate
Pyruvate oxidase	EC 1.2.3.3	Pyruvate
Pyruvate oxidase (CoA-acetylating)	EC 1.2.3.6	Pyruvate
Reticuline oxidase	EC 1.21.3.3	Reticuline
retinal oxidase	EC 1.2.3.11	Retinal
Rifamycin-B oxidase	EC 1.10.3.6	rifamycin-B
Sarcosine oxidase	EC 1.5.3.1	Sarcosine
secondary-alcohol oxidase	EC 1.1.3.18	a secondary alcohol
sulfite oxidase	EC 1.8.3.1	Sulfite
superoxide dismutase	EC 1.15.1.1	Superoxide
superoxide reductase	EC 1.15.1.2	Superoxide
tetrahydroberberine oxidase	EC 1.3.3.8	(S)-tetrahydroberberine
Thiamine oxidase	EC 1.1.3.23	Thiamine
tryptophan α,β -oxidase	EC 1.3.3.10	L-tryptophan
urate oxidase (uricase, uric acid oxidase)	EC 1.7.3.3	uric acid
Vanillyl-alcohol oxidase	EC 1.1.3.38	vanillyl alcohol
Xanthine oxidase	EC 1.17.3.2	Xanthine
xylitol oxidase	EC 1.1.3.41	Xylitol

[0096] e) Autoantibody

[0097] As used herein, the phrase "autoantibody" refers to an antibody that binds to an analyte that is endogenously produced in the subject in which the antibody is produced.

[0098] f) N-Capture Antibody: cTnT Complex (C₁)(C₂) . . . (C_n)(cTnT),

[0099] As used herein, the phrase "n-capture antibody: cTnT complex" refers to a combination of at least one anti-body and cTnT, wherein the antibody and cTnT are bound by

specific, noncovalent interactions between an antigen-combining site on the antibody and a cTnT epitope.

[0100] g) Detectable Label

[0101] As used herein the term "detectable label" refers to any moiety that generates a measurable signal via optical, electrical, or other physical indication of a change of state of a molecule or molecules coupled to the moiety. Such physical indicators encompass spectroscopic, photochemical, biochemical, immunochemical, electromagnetic, radiochemi-

cal, and chemical means, such as but not limited to fluorescence, chemifluorescence, chemiluminescence, and the like. Preferred detectable labels include acridinium compounds such as an acridinium-9-carboximide having a structure according to Formula I as set forth in section B herein below, and an acridinium-9-carboxylate aryl ester having a structure according to Formula II as also set forth in section B herein below.

[0102] h) Subject

[0103] As used herein, the terms “subject” and “patient” are used interchangeably irrespective of whether the subject has or is currently undergoing any form of treatment. As used herein, the terms “subject” and “subjects” refer to any vertebrate, including, but not limited to, a mammal (e.g., cow, pig, camel, llama, horse, goat, rabbit, sheep, hamsters, guinea pig, cat, dog, rat, and mouse, a non-human primate (for example, a monkey, such as a cynomolgous monkey, chimpanzee, etc) and a human). Preferably, the subject is a human.

[0104] i) Test Sample

[0105] As used herein, the term “test sample” generally refers to a biological material being tested for and/or suspected of containing an analyte of interest and which may also include autoantibodies to cTnT. The biological material may be derived from any biological source but preferably is a biological fluid likely to contain cTnT. Examples of biological materials include, but are not limited to, stool, whole blood, serum, plasma, red blood cells, platelets, interstitial fluid, saliva, ocular lens fluid, cerebral spinal fluid, sweat, urine, ascites fluid, mucous, nasal fluid, sputum, synovial fluid, peritoneal fluid, vaginal fluid, menses, amniotic fluid, semen, soil, etc. The test sample may be used directly as obtained from the biological source or following a pretreatment to modify the character of the sample. For example, such pretreatment may include preparing plasma from blood, diluting viscous fluids and so forth. Methods of pretreatment may also involve filtration, precipitation, dilution, distillation, mixing, concentration, inactivation of interfering components, the addition of reagents, lysing, etc. If such methods of pretreatment are employed with respect to the test sample, such pretreatment methods are such that cTnT remains in the test sample at a concentration proportional to that in an untreated test sample (e.g., namely, a test sample that is not subjected to any such pretreatment method(s)).

B. IMMUNOASSAY FOR DETECTING CTNT IN A TEST SAMPLE THAT MAY CONTAIN HETEROFILIC ENDOGENOUS ANTIBODIES, AND AUTOANTIBODIES

[0106] The present disclosure relates to an immunoassay for detecting cTnT in a test sample in which other substances that may interfere with immunodetection of cTnT may be present. Such substances include for example, heterophilic endogenous antibodies, and autoantibodies against cTnT. The immunoassay of the present disclosure involves obtaining a test sample from a subject and then detecting the presence of cTnT using immunodetection while compensating for the presence of any such substances that may be present in the sample. This is achieved in part by providing n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody: cTnT complex (C₁)(C₂) . . . (C_n)(cTnT) wherein n is an integer from 1 to 10, and n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody: n-capture antibody: cTnT measurable assembly (D₁)(D₂) . . . (D_{n'})(C₁)(C₂) . . . (C_n)(cTnT), wherein n' and n

are independently an integer from 1 to 10, and antibodies C and D bind to (n+n') different epitopes of cTnT. In other words, each of n capture antibodies C binds to at least one epitope on cTnT, and each of n' detection antibodies D binds to at least one epitope on cTnT that is different than any of the epitopes to which any of the capture antibodies C bind. Typically the detection antibodies are labeled with a detectable label, which may be conjugated directly or indirectly to the detection antibodies. The antibodies can be provided, i.e. bound to a solid phase, which can be a solid support on which for example the capture antibodies are immobilized.

Immunoassay Methods

[0107] The immunoassay methods of the present disclosure can be carried out in any of a wide variety of formats. A general review of immunoassays is available in *METHODS IN CELL BIOLOGY VOLUME 37: ANTIBODIES IN CELL BIOLOGY*, Asai, ed. Academic Press, Inc. New York (1993), and *BASIC AND CLINICAL IMMUNOLOGY 7TH EDITION*, Stites & Terr, eds. (1991), which are herein incorporated by reference in its entirety. A typical heterogeneous sandwich immunoassay employs a solid phase (as a solid support) to which is bound a first (capture) antibody reactive with at least one epitope on cTnT. A second (detection) antibody is also reactive with at least one epitope on cTnT. The second antibody may be conjugated to a detectable label that provides a signal that is measured after the detection antibody binds to the captured cTnT. When a test sample containing the cTnT contacts the first antibody, the first antibody captures the cTnT. The cTnT is contacted with the second antibody resulting in the formation of an immunodetection complex consisting of the first antibody, cTnT and second antibody, and the complex is bound to the solid phase. The signal generated by the second (detection) antibody is proportional to the concentration of the cTnT as determined by the rate of formation (k_1) of the immunodetection complex versus the rate of dissociation of the immunodetection complex (k_2). Heterophilic endogenous antibodies and any autoantibodies, which if present are unpredictable as to exactly where on cTnT they will bind, can substantially interfere with binding of the first and/or second antibody, and thus with the resulting signal.

[0108] In contrast to a typical immunoassay format, immunoassays according to an exemplary embodiment of the present disclosure employ multiple capture antibodies and/or multiple detection antibodies, wherein each detection antibody binds to at least one epitope on cTnT that is different than any of the epitopes to which any of the capture antibody or antibodies bind. It will be understood that the reference to “antibodies” in the plural, with respect to capture antibodies and detection antibodies, can refer to use in the immunoassay of one type of antibody, as in for example use of one capture antibody with use of multiple detection antibodies, or use of one detection antibody with use of multiple capture antibodies. In any case, the use of multiple capture and/or detection antibodies, wherein the capture antibodies used and detection antibodies used are distinguished by a lack of binding specificity for the same epitopes on cTnT, improves the specificity of the detection, improves the quality of signal and therefore its accuracy as to cTnT amount, and decreases noise in the signal from nonspecific binding due to the presence any heterophilic endogenous antibodies and/or autoantibodies. The signal generated by the detection antibodies remains proportional to the concentration of cTnT, but is determined by the rate of formation of a new immunodetection complex: n'-de-

tection antibody: n-capture antibody: cTnT measurable assembly $(D_1)(D_2) \dots (D_n)(C_1)(C_2) \dots (C_n)(cTnT)$, versus the rate of dissociation of the new immunodetection complex. Use of more than one capture phase antibody and more than one detection antibody improves accuracy of the immunoassay by increasing the signal from specific binding to cTnT.

[0109] The methods also provide for the use of humanized immunoreagents, which overcomes any interference from heterophilic antibodies that may be present in the test sample. For example, the capture antibodies, the detection antibodies or both the capture and detection antibodies used may be humanized. Additionally, antihuman IgG antibody can be used for the detection antibodies to correct for endogenous autoantibodies to cTnT. For example, anti-human IgG may be complexed to humanized detection antibodies. A detectable label such as those described elsewhere herein, including any of the acridinium compounds described elsewhere herein, may then be conjugated to the anti-human IgG. Moreover, when used in conjunction with humanized immunoreagents, antihuman IgG provides a "universal" signal generator. Derivatized cTnT can be used to provide a soluble reagent suitable for assay standardization.

[0110] Thus, according to one embodiment, an immunoassay of the present disclosure to detect the presence of cTnT is a heterogeneous assay employing a solid phase, which can be a solid support. The immunoassay can be performed for example by immobilizing one or more capture antibodies $(C_1)(C_2) \dots (C_n)$ on the solid phase, wherein each capture antibody C_n is an exogenous capture antibody, i.e. an exogenous antibody that is reactive with at least one epitope on cTnT. Under conditions sufficient for specific binding of each antibody C_n to cTnT, the test sample suspected of containing the cTnT and which may or may not contain other interfering substances, is contacted with the capture antibodies $(C_1)(C_2) \dots (C_n)$, thus forming a n-capture antibody: cTnT complex $(C_1)(C_2) \dots (C_n)(cTnT)$. The n-capture antibody: cTnT complex $(C_1)(C_2) \dots (C_n)(cTnT)$ is contacted with n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody: n-capture antibody: cTnT measurable assembly $(D_1)(D_2) \dots (D_{n'}) (C_1)(C_2) \dots (C_n)(cTnT)$. This step is carried out under conditions sufficient for specific binding of the D antibodies to any of the cTnT that is present in the test sample. By "measurable assembly" is meant a configuration of molecules that when formed generates a signal susceptible to physical detection and/or quantification. In certain embodiments for example, the detection antibodies D may be labeled with a detectable label. The label may be directly or indirectly conjugated to the detection antibodies. For example, in an exemplary embodiment, the detection antibodies are humanized and complexed to an antihuman IgG antibody, and then the detectable label is conjugated to the antihuman IgG antibody. Any detectable label may be conjugated to the antihuman IgG antibody, including any of the acridinium compounds described elsewhere herein. Depending on the detectable label selected and detection approach used, an optical, electrical, or change-of-state signal of the assembly is measured. Use of antihuman IgG antibody in the detection antibody corrects for endogenous autoantibodies to cTnT.

[0111] Although the immunoassay is described above as including a sequence of steps for illustrative purposes, the test sample may be contacted with the capture antibodies C and the detection antibodies D simultaneously or sequentially, in any order.

[0112] In one format of a sandwich immunoassay according to the present disclosure, detecting comprises detecting a signal from the solid phase-affixed immunodetection complex which is a n'-detection antibody: n-capture antibody: cTnT measurable assembly $(D_1)(D_2) \dots (D_{n'}) (C_1)(C_2) \dots (C_n)(cTnT)$. In one embodiment, the immunodetection complex is separated from the solid phase, typically by washing, and the signal from the bound label is detected. In another format of a sandwich immunoassay according to the present disclosure, the immunodetection complex remains a solid phase-affixed complex, which is then detected.

Antibodies

[0113] In the immunoassays according to the present disclosure, each capture antibody C can be a polyclonal antibody, a monoclonal antibody, a chimeric antibody, a human antibody, an affinity matured antibody or an antibody fragment. Similarly, each detection antibody D can be a polyclonal antibody, a monoclonal antibody, a chimeric antibody, a human antibody, an affinity matured antibody or an antibody fragment.

[0114] In an exemplary embodiment of the immunoassays, the capture antibodies, the detection antibodies or both the capture antibodies and detection antibodies are humanized. In another exemplary embodiment, the detection antibodies are humanized and complexed to an antihuman IgG antibody. The detectable label may be conjugated to the antihuman IgG antibody.

[0115] While monoclonal antibodies are highly specific to the analyte/antigen, a polyclonal antibody can preferably be used as each capture antibody C to immobilize as much of the analyte/antigen as possible. A monoclonal antibody with inherently higher binding specificity for the analyte/antigen may then preferably be used for each detection antibody D. In any case, the capture and detection antibodies recognize non-overlapping epitopes on cTnT, and in an exemplary embodiment are capable of binding simultaneously to different epitopes on cTnT, each without interfering with the binding of the other.

[0116] Polyclonal antibodies are raised by injecting (e.g., subcutaneous or intramuscular injection) an immunogen into a suitable non-human mammal (e.g., a mouse or a rabbit). Generally, the immunogen should induce production of high titers of antibody with relatively high affinity for the target antigen.

[0117] If desired, the antigen may be conjugated to a carrier protein by conjugation techniques that are well known in the art. Commonly used carriers include keyhole limpet hemocyanin (KLH), thyroglobulin, bovine serum albumin (BSA), and tetanus toxoid. The conjugate is then used to immunize the animal.

[0118] The antibodies are then obtained from blood samples taken from the animal. The techniques used to produce polyclonal antibodies are extensively described in the literature (see, e.g., *Methods of Enzymology*, "Production of Antisera With Small Doses of Immunogen: Multiple Intradermal Injections," Langone, et al. eds. (Acad. Press, 1981)). Polyclonal antibodies produced by the animals can be further purified, for example, by binding to and elution from a matrix to which the target antigen is bound. Those of skill in the art will know of various techniques common in the immunology arts for purification and/or concentration of polyclonal, as

well as monoclonal, antibodies (see, e.g., Coligan, et al. (1991) Unit 9, *Current Protocols in Immunology*, Wiley Interscience).

[0119] For many applications, monoclonal antibodies (mAbs) are preferred. The general method used for production of hybridomas secreting mAbs is well known (Kohler and Milstein (1975) *Nature*, 256:495). Briefly, as described by Kohler and Milstein, the technique entailed isolating lymphocytes from regional draining lymph nodes of five separate cancer patients with either melanoma, teratocarcinoma or cancer of the cervix, glioma or lung, (where samples were obtained from surgical specimens), pooling the cells, and fusing the cells with SHFP-1. Hybridomas were screened for production of antibody that bound to cancer cell lines. Confirmation of specificity among mAbs can be accomplished using routine screening techniques (such as the enzyme-linked immunosorbent assay, or "ELISA") to determine the elementary reaction pattern of the mAb of interest.

[0120] As used herein, the term "antibody" encompasses antigen-binding antibody fragments, e.g., single chain antibodies (scFv or others), which can be produced/selected using phage display technology. The ability to express antibody fragments on the surface of viruses that infect bacteria (bacteriophage or phage) makes it possible to isolate a single binding antibody fragment, e.g., from a library of greater than 10^{10} nonbinding clones. To express antibody fragments on the surface of phage (phage display), an antibody fragment gene is inserted into the gene encoding a phage surface protein (e.g., pIII) and the antibody fragment-pIII fusion protein is displayed on the phage surface (McCafferty et al. (1990) *Nature*, 348: 552-554; Hoogenboom et al. (1991) *Nucleic Acids Res.* 19: 4133-4137).

[0121] Since the antibody fragments on the surface of the phage are functional, phage-bearing antigen-binding antibody fragments can be separated from non-binding phage by antigen affinity chromatography (McCafferty et al. (1990) *Nature*, 348: 552-554). Depending on the affinity of the antibody fragment, enrichment factors of 20-fold-1,000,000-fold are obtained for a single round of affinity selection. By infecting bacteria with the eluted phage, however, more phage can be grown and subjected to another round of selection. In this way, an enrichment of 1000-fold in one round can become 1,000,000-fold in two rounds of selection (McCafferty et al. (1990) *Nature*, 348: 552-554). Thus, even when enrichments are low (Marks et al. (1991) *J. Mol. Biol.* 222: 581-597), multiple rounds of affinity selection can lead to the isolation of rare phage. Since selection of the phage antibody library on antigen results in enrichment, the majority of clones bind antigen after as few as three to four rounds of selection. Thus only a relatively small number of clones (several hundred) need to be analyzed for binding to antigen. Human antibodies can be produced without prior immunization by displaying very large and diverse V-gene repertoires on phage (Marks et al. (1991) *J. Mol. Biol.* 222: 581-597). In one embodiment, natural VH and VL repertoires present in human peripheral blood lymphocytes are isolated from unimmunized donors by PCR. The V-gene repertoires can be spliced together at random using PCR to create a scFv gene repertoire which can be cloned into a phage vector to create a library of 30 million phage antibodies (Id.). From a single "naive" phage antibody library, binding antibody fragments have been isolated against more than 17 different antigens, including haptens, polysaccharides, and proteins (Marks et al. (1991) *J. Mol. Biol.* 222: 581-597; Marks et al. (1993) *Bio/Technology*, 10:

779-783; Griffiths et al. (1993) *EMBO J.* 12: 725-734; Clackson et al. (1991) *Nature*. 352: 624-628). Antibodies have been produced against self proteins, including human thyroglobulin, immunoglobulin, tumor necrosis factor, and CEA (Griffiths et al. (1993) *EMBO J.* 12: 725-734). The antibody fragments are highly specific for the antigen used for selection and have affinities in the 1 nM to 100 nM range (Marks et al. (1991) *J. Mol. Biol.* 222: 581-597; Griffiths et al. (1993) *EMBO J.* 12: 725-734). Larger phage antibody libraries result in the isolation of more antibodies of higher binding affinity to a greater proportion of antigens.

[0122] As those of skill in the art readily appreciate, antibodies can be prepared by any of a number of commercial services (e.g., Berkeley Antibody Laboratories, Bethyl Laboratories, Anawa, Eurogenetec, etc.).

Solid Phase

[0123] A solid phase can be any suitable material with sufficient surface affinity to bind an antibody, for example each capture antibody C. The solid phase can take any of a number of forms, such as a magnetic particle, bead, test tube, microtiter plate, cuvette, membrane, a scaffolding molecule, quartz crystal, film, filter paper, disc or a chip. Useful solid phase materials include: natural polymeric carbohydrates and their synthetically modified, crosslinked, or substituted derivatives, such as agar, agarose, cross-linked alginic acid, substituted and cross-linked guar gums, cellulose esters, especially with nitric acid and carboxylic acids, mixed cellulose esters, and cellulose ethers; natural polymers containing nitrogen, such as proteins and derivatives, including cross-linked or modified gelatins; natural hydrocarbon polymers, such as latex and rubber; synthetic polymers, such as vinyl polymers, including polyethylene, polypropylene, polystyrene, polyvinylchloride, polyvinylacetate and its partially hydrolyzed derivatives, polyacrylamides, polymethacrylates, copolymers and terpolymers of the above polycondensates, such as polyesters, polyamides, and other polymers, such as polyurethanes or polyepoxides; inorganic materials such as sulfates or carbonates of alkaline earth metals and magnesium, including barium sulfate, calcium sulfate, calcium carbonate, silicates of alkali and alkaline earth metals, aluminum and magnesium; and aluminum or silicon oxides or hydrates, such as clays, alumina, talc, kaolin, zeolite, silica gel, or glass (these materials may be used as filters with the above polymeric materials); and mixtures or copolymers of the above classes, such as graft copolymers obtained by initializing polymerization of synthetic polymers on a pre-existing natural polymer. All of these materials may be used in suitable shapes, such as films, sheets, tubes, particulates, or plates, or they may be coated onto, bonded, or laminated to appropriate inert carriers, such as paper, glass, plastic films, fabrics, or the like. Nitrocellulose has excellent absorption and adsorption qualities for a wide variety of reagents including monoclonal antibodies. Nylon also possesses similar characteristics and also is suitable.

[0124] Alternatively, the solid phase can constitute microparticles. Microparticles useful in the present disclosure can be selected by one skilled in the art from any suitable type of particulate material and include those composed of polystyrene, polymethylacrylate, polypropylene, latex, polytetrafluoroethylene, polyacrylonitrile, polycarbonate, or similar materials. Further, the microparticles can be magnetic or paramagnetic microparticles, so as to facilitate manipulation

of the microparticle within a magnetic field. In an exemplary embodiment the microparticles are carboxylated magnetic microparticles.

[0125] Microparticles can be suspended in the mixture of soluble reagents and test sample or can be retained and immobilized by a support material. In the latter case, the microparticles on or in the support material are not capable of substantial movement to positions elsewhere within the support material. Alternatively, the microparticles can be separated from suspension in the mixture of soluble reagents and test sample by sedimentation or centrifugation. When the microparticles are magnetic or paramagnetic the microparticles can be separated from suspension in the mixture of soluble reagents and test sample by a magnetic field.

[0126] The methods of the present disclosure can be adapted for use in systems that utilize microparticle technology including automated and semi-automated systems wherein the solid phase comprises a microparticle. Such systems include those described in pending U.S. App. No. 425, 651 and U.S. Pat. No. 5,089,424, which correspond to published EPO App. Nos. EP 0 425 633 and EP 0 424 634, respectively, and U.S. Pat. No. 5,006,309.

[0127] In particular embodiments, the solid phase includes one or more electrodes. Capture antibodies C can be affixed for example, directly or indirectly, to the electrode(s). In one embodiment, for example, capture antibodies C can be affixed to magnetic or paramagnetic microparticles, which are then positioned in the vicinity of the electrode surface using a magnet. Systems in which one or more electrodes serve as the solid phase are useful where detection is based on electrochemical interactions. Exemplary systems of this type are described, for example, in U.S. Pat. No. 6,887,714 (issued May 3, 2005). The basic method is described further below with respect to electrochemical detection.

[0128] The capture antibodies C can be attached to the solid phase by adsorption, where they are retained by hydrophobic forces. Alternatively, the surface of the solid phase can be activated by chemical processes that cause covalent linkage of the capture antibodies to the support.

[0129] To change or enhance the intrinsic charge of the solid phase, a charged substance can be coated directly onto the solid phase. Ion capture procedures for immobilizing an immobilizable reaction complex with a negatively charged polymer, described in U.S. App. No. 150,278, corresponding to EP Publication No. 0326100, and U.S. App. No. 375,029 (EP Publication No. 0406473), can be employed according to the present disclosure to affect a fast solution-phase immunochemical reaction. In these procedures, an immobilizable immune complex is separated from the rest of the reaction mixture by ionic interactions between the negatively charged polyanion/immune complex and the previously treated, positively charged matrix and detected by using any of a number of signal-generating systems, including, e.g., chemiluminescent systems, as described in U.S. App. No. 921,979, corresponding to EPO Publication No. 0 273,115.

[0130] If the solid phase is silicon or glass, the surface must generally be activated prior to attaching each capture antibody C. Activated silane compounds such as triethoxy amino propyl silane (available from Sigma Chemical Co., St. Louis, Mo.), triethoxy vinyl silane (Aldrich Chemical Co., Milwaukee, Wis.), and (3-mercaptopropyl)-trimethoxy silane (Sigma Chemical Co., St. Louis, Mo.) can be used to introduce reactive groups such as amino-, vinyl, and thiol, respectively. Such activated surfaces can be used to link the capture

directly (in the cases of amino or thiol), or the activated surface can be further reacted with linkers such as glutaraldehyde, bis(succinimidyl) suberate, SPPD 9 succinimidyl 3-[2-pyridyldithio]propionate), SMCC (succinimidyl-4-[Nmaleimidomethyl]cyclohexane-1-carboxylate), SIAB (succinimidyl[4iodoacetyl]aminobenzoate), and SMPB (succinimidyl 4-[1maleimidophenyl]butyrate) to separate the capture antibody from the surface. Vinyl groups can be oxidized to provide a means for covalent attachment. Vinyl groups can also be used as an anchor for the polymerization of various polymers such as poly-acrylic acid, which can provide multiple attachment points for specific capture antibodies. Amino groups can be reacted with oxidized dextrans of various molecular weights to provide hydrophilic linkers of different size and capacity. Examples of oxidizable dextrans include Dextran T-40 (molecular weight 40,000 daltons), Dextran T-110 (molecular weight 110,000 daltons), Dextran T-500 (molecular weight 500,000 daltons), Dextran T-2M (molecular weight 2,000,000 daltons) (all of which are available from Pharmacia, Piscataway, N.J.), or Ficoll (molecular weight 70,000 daltons; available from Sigma Chemical Co., St. Louis, Mo.). Additionally, polyelectrolyte interactions can be used to immobilize a specific capture antibody on a solid phase using techniques and chemistries described U.S. App. No. 150,278, filed Jan. 29, 1988, and U.S. App. No. 375,029, filed Jul. 7, 1989, each of which is incorporated herein by reference.

[0131] Other considerations affecting the choice of solid phase include the ability to minimize non-specific binding of labeled entities and compatibility with the labeling system employed. For, example, solid phases used with fluorescent labels should have sufficiently low background fluorescence to allow signal detection.

[0132] Following attachment of a specific capture antibody, the surface of the solid support may be further treated with materials such as serum, proteins, or other blocking agents to minimize non-specific binding.

Detection Systems in General

[0133] As discussed above, immunoassays according to the present disclosure employ one or more detection antibodies D, each of which is cTnT-specific. In certain embodiments, each detection antibody D has a detectable label.

[0134] Detectable labels suitable for use in the detection antibodies of the present disclosure include any compound or composition having a moiety that is detectable by spectroscopic, photochemical, biochemical, immunochemical, electrical, optical, or chemical means. Such labels include, for example, an enzyme, oligonucleotide, nanoparticle chemilumiphore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin. Thus for example, in an immunoassay employing an optical signal, the optical signal is measured as an analyte concentration dependent change in chemiluminescence, fluorescence, phosphorescence, electrochemiluminescence, ultraviolet absorption, visible absorption, infrared absorption, refraction, surface plasmon resonance. In an immunoassay employing an electrical signal, the electrical signal is measured as an analyte concentration dependent change in current, resistance, potential, mass to charge ratio, or ion count. In an immunoassay employing a change-of-state signal, the change of state signal is measured as an analyte concentration dependent change in size, solubility, mass, or resonance.

[0135] Useful labels according to the present disclosure include magnetic beads (e.g., Dynabeads™), fluorescent dyes (e.g., fluorescein, Texas Red, rhodamine, green fluorescent protein) and the like (see, e.g., Molecular Probes, Eugene, Oreg., USA), chemiluminescent compounds such as acridinium (e.g., acridinium-9-carboxamide), phenanthridinium, dioxetanes, luminol and the like, radiolabels (e.g., ³H, ¹²⁵I, ³⁵S, ¹⁴C, or ³²P), catalysts such as enzymes (e.g., horse radish peroxidase, alkaline phosphatase, beta-galactosidase and others commonly used in an ELISA), and colorimetric labels such as colloidal gold (e.g., gold particles in the 40-80 nm diameter size range scatter green light with high efficiency) or colored glass or plastic (e.g., polystyrene, polypropylene, latex, etc.) beads. Patents teaching the use of such labels include U.S. Pat. Nos. 3,817,837; 3,850,752; 3,939,350; 3,996,345; 4,277,437; 4,275,149; and 4,366,241.

[0136] The label can be attached to each detection antibody prior to, or during, or after contact with the biological sample. So-called "direct labels" are detectable labels that are directly attached to or incorporated into the detection antibody prior to use in the assay. Direct labels can be attached to or incorporated into the detection antibody by any of a number of means well known to those of skill in the art.

[0137] In contrast, so-called "indirect labels" typically bind to each detection antibody at some point during the assay. Often, the indirect label binds to a moiety that is attached to or incorporated into the detection agent prior to use. Thus, for example, each detection antibody can be biotinylated before use in an assay. During the assay, an avidin-conjugated fluorophore can bind the biotin-bearing detection agent, to provide a label that is easily detected.

[0138] In another example of indirect labeling, polypeptides capable of specifically binding immunoglobulin constant regions, such as polypeptide A or polypeptide G, can also be used as labels for detection antibodies. These polypeptides are normal constituents of the cell walls of streptococcal bacteria. They exhibit a strong non-immunogenic reactivity with immunoglobulin constant regions from a variety of species (see, generally Kronval, et al. (1973) *J. Immunol.*, 111: 1401-1406, and Akerstrom (1985) *J. Immunol.*, 135: 2589-2542). Such polypeptides can thus be labeled and added to the assay mixture, where they will bind to each capture and detection antibody, as well as to the autoantibodies, labeling all and providing a composite signal attributable to analyte and autoantibody present in the sample.

[0139] Some labels useful in the present disclosure may require the use of an additional reagent(s) to produce a detectable signal. In an ELISA, for example, an enzyme label (e.g., beta-galactosidase) will require the addition of a substrate (e.g., X-gal) to produce a detectable signal. In immunoassays using an acridinium compound as the direct label, a basic solution and a source of hydrogen peroxide are added.


Detection Systems—Exemplary Formats

[0140] Chemiluminescence Immunoassay: In an exemplary embodiment, a chemiluminescent compound is used in the above-described methods as a direct label conjugated to each detection antibody D. The chemiluminescent compound can be an acridinium compound. When an acridinium compound is used as the detectable label, then the above-described method may further include generating or providing a source of hydrogen peroxide to the mixture resulting from contacting the test sample with the first antibody and the second antibody, and adding at least one basic solution to the

mixture to generate a light signal. The light signal generated or emitted by the mixture is then measured to detect cTnT in the test sample.

[0141] The source of hydrogen peroxide may be a buffer solution or a solution containing hydrogen peroxide or an enzyme that generates hydrogen peroxide when added to the test sample. The basic solution serves as a trigger solution, and the order in which the at least one basic solution and detectable label are added is not critical. The basic solution used in the method is a solution that contains at least one base and that has a pH greater than or equal to 10, preferably, greater than or equal to 12. Examples of basic solutions include, but are not limited to, sodium hydroxide, potassium hydroxide, calcium hydroxide, ammonium hydroxide, magnesium hydroxide, sodium carbonate, sodium bicarbonate, calcium hydroxide, calcium carbonate and calcium bicarbonate. The amount of basic solution added to the test sample depends on the concentration of the basic solution used in the assay. Based on the concentration of the basic solution used, one skilled in the art could easily determine the amount of basic solution to be used in the method described herein.

[0142] In a chemiluminescence immunoassay according to the present disclosure and using an acridinium compound as the detectable label, preferably the acridinium compound is an acridinium-9-carboxamide. Specifically, the acridinium-9-carboxamide has a structure according to formula I:

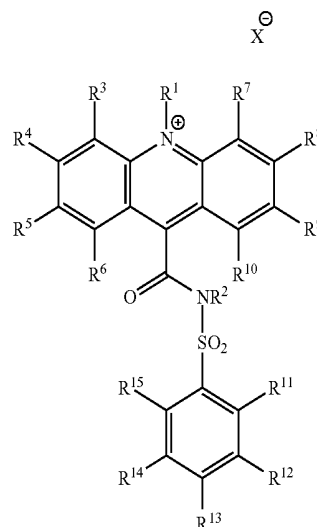

[0143] wherein R¹ and R² are each independently selected from the group consisting of: alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl, and


[0144] wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and further wherein any of the alkyl, alkenyl, alkynyl, aryl or aralkyl may contain one or more heteroatoms; and

[0145] optionally, if present, X[⊖] is an anion.

[0146] Methods for preparing acridinium 9-carboxamides are described in Mattingly, P. G. *J. Biolumin. Chemilumin.*, 6, 107-14; (1991); Adamczyk, M.; Chen, Y.-Y., Mattingly, P. G.; Pan, Y. *J. Org. Chem.*, 63, 5636-5639 (1998); Adamczyk, M.;

Chen, Y.-Y.; Mattingly, P. G.; Moore, J. A.; Shreder, K. *Tetrahedron*, 55, 10899-10914 (1999); Adamczyk, M.; Mattingly, P. G.; Moore, J. A.; Pan, Y. *Org. Lett.*, 1, 779-781 (1999); Adamczyk, M.; Chen, Y.-Y.; Fishpaugh, J. R.; Mattingly, P. G.; Pan, Y.; Shreder, K.; Yu, Z. *Bioconjugate Chem.*, 11, 714-724 (2000); Mattingly, P. G.; Adamczyk, M. In *Luminescence Biotechnology: Instruments and Applications*; Dyke, K. V. Ed.; CRC Press: Boca Raton, pp. 77-105 (2002); Adamczyk, M.; Mattingly, P. G.; Moore, J. A.; Pan, Y. *Org. Lett.*, 5, 3779-3782 (2003); and U.S. Pat. Nos. 5,468,646, 5,543,524 and 5,783,699 (each incorporated herein by reference in their entireties for their teachings regarding same).

[0147] Alternatively, the acridinium compound can be an acridinium-9-carboxylate aryl ester; the acridinium-9-carboxylate aryl ester can have a structure according to formula II:

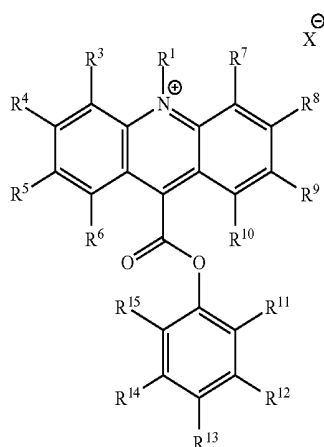

[0148] wherein R¹ is an alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0149] wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0150] optionally, if present, X[⊖] is an anion.

[0151] Examples of acridinium-9-carboxylate aryl esters having the above formula II that can be used in the present disclosure include, but are not limited to, 10-methyl-9-(phenoxycarbonyl)acridinium fluorosulfonate (available from Cayman Chemical, Ann Arbor, Mich.). Methods for preparing acridinium 9-carboxylate aryl esters are described in McCapra, F., et al., *Photochem. Photobiol.*, 4, 1111-21 (1965); Razavi, Z et al., *Luminescence*, 15:245-249 (2000); Razavi, Z et al., *Luminescence*, 15:239-244 (2000); and U.S. Pat. No. 5,241,070 (each incorporated herein by reference in their entireties for their teachings regarding same).

[0152] In addition to the at least one acridinium compound, the indicator solution can also contain at least one surfactant. Any surfactant that when dissolved in water, lowers the surface tension of the water and increases the solubility of organic compounds, can be used in the present invention. Examples of surfactants that can be used is one or more non-ionic or ionic surfactants (e.g., anionic, cationic or zwitterionic surfactants). Examples of non-ionic surfactants that can be used include, but are not limited to, t-octylphoxypoly-

ethoxyethanol (TRITON X-100, Sigma Aldrich, St. Louis, Mo.), polyoxyethylenesorbitan monolaurate (Tween 20), nonylphenol polyoxyethylene ether (Nonidet P10), decyldimethylphosphine oxide (APO-10), Cyclohexyl-n-ethyl-β-D-Maltoside, Cyclohexyl-n-hexyl-β-D-Maltoside, Cyclohexyl-n-methyl-β-D-Maltoside, n-Decanoylsucrose, n-Decyl-β-D-glucopyranoside, n-Decyl-β-D-maltopyranoside, n-Decyl-β-D-thiomaltoside, Digitonin, n-Dodecanoyl sucrose, n-Dodecyl-β-D-glucopyranoside, n-Dodecyl-β-D-maltoside, polyoxyethylene (10) dodecyl ether (Genapol C-100), isotridecanol polyglycol ether (Genapol X-80), isotridecanol polyglycol ether (Genapol X-100), Heptane-1,2,3-triol, n-Heptyl-β-D-glucopyranoside, n-Heptyl-β-D-thiogluco-pyranoside and combinations thereof. An example of an ionic surfactant that can be used include, sodium cholate, chenodeoxycholic acid, cholic acid, dehydrocholic acid, docusate sodium, docusate sodium salt, glycocholic acid hydrate, glycodeoxycholic acid monohydrate, glycolithocholic acid ethyl ester, N-lauroylsarcosine sodium salt, N-lauroylsarcosine, lithium dodecyl sulfate, calcium propionate, 1-octanesulfonic acid sodium salt, sodium 1-butanesulfonate, sodium chenodeoxycholate, sodium cholate hydrate, sodium 1-decanesulfonate, sodium 1-decanesulfonate, sodium deoxycholate, sodium deoxycholate monohydrate, sodium dodecylbenzenesulfonate, sodium dodecyl sulfate, sodium glycochenodeoxycholate, sodium glycocholate hydrate, sodium 1-heptanesulfonate, sodium hexanesulfonate, sodium 1-nonanesulfonate, sodium octyle sulfate, sodium pentanesulfonate, sodium 1-propanesulfonate hydrate, sodium taurodeoxycholate hydrate, sodium taurohydrodeoxycholate hydrate, sodium taurooursodeoxycholate, taurocholic acid sodium salt hydrate, tauroolithocholic acid 3-sulfate disodium salt, Triton® X-200, Triton® QS-15, Triton® QS-44, Triton® XQS-20, Trizma® dodecyl sulfate, ursodeoxycholic acid, alkyltrimethylammonium bromide, amprolium hydrochloride, benzalkonium chloride, benzethonium hydroxide, benzyltrimethylhexadecylammonium chloride, benzyltrimethylhexadecylammonium bromide, choline p-toluenesulfonate salt, dimethyldioctadecylammonium bromide, dodecylethyltrimethylammonium bromide, dodecyltrimethylammonium bromide, ethylhexadecyltrimethylammonium bromide, Ggirard's reagent, hexadecylpyridinium bromide, hexadecylpyridinium chloride monohydrate, hexadecylpyridinium chloride monohydrate, hexadecyltrimethylammonium bromide, hexadecyltrimethylammonium p-toluenesulfonate, hexadecyltrimethylammonium bromide, hexadecyltrimethylammonium p-toluenesulfonate, Hyamine® 1622, methylbenzethonium chloride, myristyltrimethylammonium bromide, oxyphenonium bromide, N,N',N'-polyoxyethylene (10)-N-tallow-1,3-diaminopropane, tetraheptylammonium bromide, tetrakis(decyl)ammonium bromide, thonzonium bromide and Luviquat™ FC370, Luviquat™ HM 552, Luviquat™ HOLD, Luviquat™ MS 370, Luviquat™ PQ 11PN and combinations thereof (all available from Sigma Aldrich, St. Louis, Mo.).

[0153] Optionally, the test sample may be treated prior to the addition of any one or more of the at least one basic solution, hydrogen peroxide source and detectable label. Such treatment may include dilution, ultrafiltration, extraction, precipitation, dialysis, chromatography and digestion. Such treatment may be in addition to and separate from any pretreatment that the test sample may receive or be subjected to as discussed previously herein. Moreover, if such treatment methods are employed with respect to the test sample, such

treatment methods are such that cTnT remains in the test sample at a concentration proportional to that in an untreated test sample (e.g., namely, a test sample that is not subjected to any such treatment method(s)).

[0154] As mentioned briefly previously herein, the time and order in which the test sample, the at least one basic solution, source of hydrogen peroxide and the detectable label are added to form a mixture is not critical. Additionally, the mixture formed by the at least one basic solution, hydrogen peroxide source and the detectable label, can optionally be allowed to incubate for a period of time. For example, the mixture can be allowed to incubate for a period of time of from about 1 second to about 60 minutes. Specifically, the mixture can be allowed to incubate for a period of from about 1 second to about 18 minutes.

[0155] When a chemiluminescent detectable label is used, after the addition of the at least one basic solution, hydrogen peroxide source, and the detectable label to the test sample, a detectable signal, namely, a chemiluminescent signal, is generated. The signal generated by the mixture is detected for a fixed duration of time. Preferably, the mixture is formed and the signal is detected concurrently. The duration of the detection may range from about 0.01 to about 360 seconds, more preferably from about 0.1 to about 30 seconds, and most preferably from about 0.5 to about 5 seconds. Chemiluminescent signals generated can be detected using routine techniques known to those skilled in the art.

[0156] Thus, in a chemiluminescent immunoassay according to the present disclosure, a chemiluminescent detectable label is used and added to the test sample, the chemiluminescent signal generated after the addition of the basic solution and the detectable label indicates the presence of cTnT in the test sample, which signal can be detected. The amount or concentration of cTnT in the test sample can be quantified based on the intensity of the signal generated. Specifically, the amount of cTnT contained in a test sample is proportional to the intensity of the signal generated. Specifically, the amount of cTnT present can be quantified based on comparing the amount of light generated to a standard curve for cTnT or by comparison to a cTnT reference standard. The cTnT reference standard may comprise, for example, an anti-idiotypic antibody. The cTnT reference standard may comprise for example a derivatized cTnT, such as for example cTnT derivatized with a polyethylene glycol. The standard curve can be generated using serial dilutions or solutions to cTnT of known concentration, by mass spectroscopy, gravimetrically and by other techniques known in the art. The above kit may further comprise a cTnT reference standard.

[0157] Fluorescence Polarization Immunoassay (FPIA): In an exemplary embodiment, a fluorescent label is employed in a fluorescence polarization immunoassay (FPIA) according to the invention. Generally, fluorescent polarization techniques are based on the principle that a fluorescent label, when excited by plane-polarized light of a characteristic wavelength, will emit light at another characteristic wavelength (i.e., fluorescence) that retains a degree of the polarization relative to the incident light that is inversely related to the rate of rotation of the label in a given medium. As a consequence of this property, a label with constrained rotation, such as one bound to another solution component with a relatively lower rate of rotation, will retain a relatively greater degree of polarization of emitted light than when free in solution.

[0158] This technique can be employed in immunoassays according to the invention, for example, by selecting reagents such that binding of the fluorescently labeled entities forms a complex sufficiently different in size such that a change in the intensity light emitted in a given plane can be detected. For example, when a labeled cardiac troponin antibody is bound by one or more cardiac troponin antigens captured by the capture antibody and/or autoantibodies reactive with the cardiac troponin, the resulting complex is sufficiently larger, and its rotation is sufficiently constrained, relative to the free labeled cardiac troponin antibody that binding is easily detected.

[0159] Fluorophores useful in FPIA include fluorescein, aminofluorescein, carboxyfluorescein, and the like, preferably 5 and 6-aminomethylfluorescein, 5 and 6-aminofluorescein, 6-carboxyfluorescein, 5-carboxyfluorescein, thioureafluorescein, and methoxytriazinyl-aminofluorescein, and similar fluorescent derivatives. Examples of commercially available automated instruments with which fluorescence polarization assays can be conducted include: the IMx system, the TDx system, and TDxFLx system (all available from Abbott Laboratories, Abbott Park, Ill.).

[0160] Scanning Probe Microscopy (SPM): The use of scanning probe microscopy (SPM) for immunoassays also is a technology to which the immunoassay methods of the present disclosure are easily adaptable. In SPM, in particular in atomic force microscopy, the capture antibody is affixed to the solid phase that in addition to being capable of binding autoantibodies, has a surface suitable for scanning. The capture antibody can, for example, be adsorbed to a plastic or metal surface. Alternatively, the capture antibody can be covalently attached to, e.g., derivatized plastic, metal, silicon, or glass according to methods known to those of ordinary skill in the art. Following attachment of the capture antibody, the test sample is contacted with the solid phase, and a scanning probe microscope is used to detect and quantify solid phase-affixed complexes. The use of SPM eliminates the need for labels that are typically employed in immunoassay systems. Such a system is described in U.S. App. No. 662,147, which is incorporated herein by reference.

[0161] MicroElectroMechanical Systems (MEMS): Immunoassays according to the present disclosure can also be carried out using a MicroElectroMechanical System (MEMS). MEMS are microscopic structures integrated onto silicon that combine mechanical, optical, and fluidic elements with electronics, allowing convenient detection of an analyte of interest. An exemplary MEMS device suitable for use in the present disclosure is the Protiveris' multicantilever array. This array is based on chemo-mechanical actuation of specially designed silicon microcantilevers and subsequent optical detection of the microcantilever deflections. When coated on one side with a binding partner, a microcantilever will bend when it is exposed to a solution containing the complementary molecule. This bending is caused by the change in the surface energy due to the binding event. Optical detection of the degree of bending (deflection) allows measurement of the amount of complementary molecule bound to the microcantilever.

[0162] Electrochemical Detection Systems: In other embodiments, immunoassays according to the present disclosure are carried out using electrochemical detection, the techniques for which are well known to those skilled in the art. Such electrochemical detection often employs one or more electrodes connected to a device that measures and records an

electrical current. Such techniques can be realized in a number of commercially available devices, such as the I-STAT® (Abbott Laboratories, Abbott Park, Ill.) system, which comprises a hand-held electrochemical detection instrument and self-contained assay-specific reagent cartridges. For example, in the present invention, the basic trigger solution could be contained in the self-contained hemoglobin reagent cartridge and upon addition of the test sample, a current would be generated at least one electrode that is proportional to the amount of hemoglobin in the test sample. A basic procedure for electrochemical detection has been described for example by Heineman and coworkers. This entailed immobilization of a primary antibody (Ab, rat-anti mouse IgG), followed by exposure to a sequence of solutions containing the antigen (Ag, mouse IgG), the secondary antibody conjugated to an enzyme label (AP-Ab, rat anti mouse IgG and alkaline phosphatase), and p-aminophenyl phosphate (PAPP). The AP converts PAPP to p-aminophenol (PAP_R, the "R" is intended to distinguish the reduced form from the oxidized form, PAP_O, the quinoneimine), which is electrochemically reversible at potentials that do not interfere with reduction of oxygen and water at pH 9.0, where AP exhibits optimum activity. PAP_R does not cause electrode fouling, unlike phenol whose precursor, phenylphosphate, is often used as the enzyme substrate. Although PAP_R undergoes air and light oxidation, these are easily prevented on small scales and short time frames. Picomole detection limits for PAP_R and femtogram detection limits for IgG achieved in micro-electrochemical immunoassays using PAPP volumes ranging from 20 μl to 360 μL have been reported previously. In capillary immunoassays with electrochemical detection, the lowest detection limit reported thus far is 3000 molecules of mouse IgG using a volume of 70 μL and a 30 min or 25 min assay time.

[0163] In an exemplary embodiment employing electrochemical detection according to the present disclosure, a capture antibody reactive with cTnT can be immobilized on the surface of an electrode which is the solid phase. The electrode is then contacted with a test sample from, e.g., a human. Any analyte in the sample binds to the capture antibody to form a first solid phase-affixed complex. Autoantibodies also bind to the surface of the electrode thereby becoming immobilized on the surface of the electrode. Analyte in the test sample that is unbound by the capture antibody binds to immobilized autoantibodies that are reactive with the analyte to form a second solid phase-affixed complex. These solid phase-affixed complexes are contacted with a detection antibody that is analyte-specific and has a detectable label. Formation of an immunodetection complex including the first antibody-analyte-second antibody complex plus the autoantibody-analyte-second antibody complex results in generation of a signal by the detectable label, which is then detected.

[0164] Various electrochemical detection systems are described in U.S. Pat. No. 7,045,364 (issued May 16, 2006; incorporated herein by reference), U.S. Pat. No. 7,045,310 (issued May 16, 2006; incorporated herein by reference), U.S. Pat. No. 6,887,714 (issued May 3, 2005; incorporated herein by reference), U.S. Pat. No. 6,682,648 (issued Jan. 27, 2004; incorporated herein by reference); U.S. Pat. No. 6,670,115 (issued Dec. 30, 2003; incorporated herein by reference).

C. KITS


[0165] The present disclosure also provides kits for assaying test samples for presence of cTnT wherein the test sample

may contain other substances that interfere with immunodetection of cTnT. Kits according to the present disclosure include one or more reagents useful for practicing one or more immunoassays according to the present disclosure. A kit generally includes a package with one or more containers holding the reagents, as one or more separate compositions or, optionally, as admixture where the compatibility of the reagents will allow. The test kit can also include other material(s), which may be desirable from a user standpoint, such as a buffer(s), a diluent(s), a standard(s), and/or any other material useful in sample processing, washing, or conducting any other step of the assay.

[0166] In certain embodiments, a test kit includes a humanized monoclonal antibody, wherein the humanized monoclonal antibody is specific for cTnT. This component can be used as a positive control in immunoassays according to the invention. If desired, this component can be included in the test kit in multiple concentrations to facilitate the generation of a standard curve to which the signal detected in the test sample can be compared. Alternatively, a standard curve can be generated by preparing dilutions of a single humanized monoclonal antibody solution provided in the kit.

[0167] Kits according to the present disclosure can include one or more capture antibodies C, each of which binds to at least one epitope on cTnT, and one or more detection antibodies D, each of which binds to at least one epitope on cTnT that is different from any epitope to which any of the capture antibodies bind, and instructions for detecting or quantifying cTnT. In certain embodiments test kits according to the present disclosure may include the solid phase, to which the capture antibodies and/or detection antibodies are bound. The solid phase may be a material such as a magnetic particle, a bead, a test tube, a microtiter plate, a cuvette, a membrane, a scaffolding molecule, a quartz crystal, a film, a filter paper, a disc or a chip.

[0168] Test kits according to the present disclosure can include for example non-human monoclonal antibodies against cTnT, as the capture and detection antibodies. The kit may also include a detectable label that can be or is conjugated to each detection antibody. In certain embodiments, the test kit includes at least one direct label, which may be an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin. In some embodiments, the direct label is an acridinium compound such as an acridinium-9-carboxamide according to formula I:

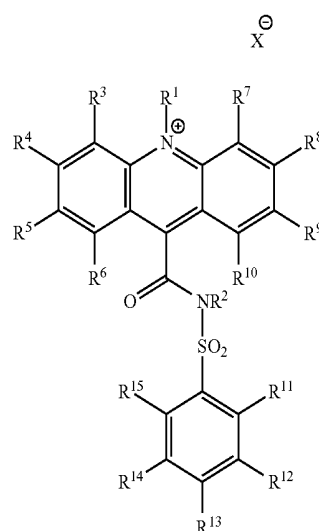


I

[0169] wherein R^1 and R^2 are each independently selected from the group consisting of: alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl, and

[0170] wherein R^3 through R^{15} are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and optionally, if present, X^\ominus is an anion.

[0171] Alternatively, the acridinium compound can be an acridinium-9-carboxylate aryl ester having a structure according to formula II:

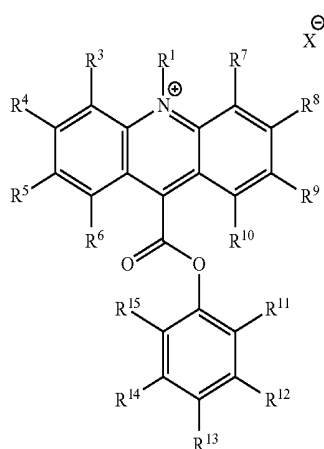

[0172] wherein R^1 is an alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0173] wherein R^3 through R^{15} are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and

[0174] optionally, if present, X^\ominus is an anion.

[0175] Test kits according to the present disclosure and which include an acridinium compound can also include a basic solution. For example, the basic solution can be a solution having a pH of at least about 10.

[0176] In certain embodiments, test kits according to the present disclosure may further include a hydrogen peroxide source, such as a buffer solution, a solution containing hydrogen peroxide, or a hydrogen peroxide generating enzyme. For example, test kits may include an amount of a hydrogen peroxide generating enzymes selected from the following: (R)-6-hydroxynicotine oxidase, (S)-2-hydroxy acid oxidase, (S)-6-hydroxynicotine oxidase, 3-aci-nitropropanoate oxidase, 3-hydroxyanthranilate oxidase, 4-hydroxymandelate oxidase, 6-hydroxynicotinate dehydrogenase, abscisic-aldehyde oxidase, acyl-CoA oxidase, alcohol oxidase, aldehyde oxidase, amine oxidase, amine oxidase (copper-containing), amine oxidase (flavin-containing), aryl-alcohol oxidase, aryl-aldehyde oxidase, catechol oxidase, cholesterol oxidase, choline oxidase, columbamine oxidase, cyclohexylamine oxidase, cytochrome c oxidase, D-amino-acid oxidase, D-arabinono-1,4-lactone oxidase, D-arabinono-1,4-lactone oxidase, D-aspartate oxidase, D-glutamate oxidase, D-glutamate(D-aspartate) oxidase, dihydrobenzophenanthridine oxidase, dihydroorotate oxidase, dihydrouracil oxidase, dimethylglycine oxidase, D-mannitol oxidase, ecdysone oxi-

dase, ethanolamine oxidase, galactose oxidase, glucose oxidase, glutathione oxidase, glycerol-3-phosphate oxidase, glycine oxidase, glyoxylate oxidase, hexose oxidase, hydroxyphytanate oxidase, indole-3-acetaldehyde oxidase, lactic acid oxidase, L-amino-acid oxidase, L-aspartate oxidase, L-galactonolactone oxidase, L-glutamate oxidase, L-gulonolactone oxidase, L-lysine 6-oxidase, L-lysine oxidase, long-chain-alcohol oxidase, L-pipecolate oxidase, L-sorbose oxidase, malate oxidase, methanethiol oxidase, monoamino acid oxidase, N6-methyl-lysine oxidase, N-acyl-hexosamine oxidase, NAD(P)H oxidase, nitroalkane oxidase, N-methyl-L-amino-acid oxidase, nucleoside oxidase, oxalate oxidase, polyamine oxidase, polyphenol oxidase, polyvinyl-alcohol oxidase, prenylcysteine oxidase, protein-lysine 6-oxidase, putrescine oxidase, pyranose oxidase, pyridoxal 5'-phosphate synthase, pyridoxine 4-oxidase, pyrroloquinoline-quinone synthase, pyruvate oxidase, pyruvate oxidase (CoA-acetylating), reticuline oxidase, retinal oxidase, rifamycin-B oxidase, sarcosine oxidase, secondary-alcohol oxidase, sulfite oxidase, superoxide dismutase, superoxide reductase, tetrahydroberberine oxidase, thiamine oxidase, tryptophan α,β -oxidase, urate oxidase (uricase, uric acid oxidase), vanillyl-alcohol oxidase, xanthine oxidase, xylitol oxidase and combinations thereof.

[0177] Test kits according to the present disclosure preferably include instructions for carrying out one or more of the immunoassays of the invention. Instructions included in kits of the present disclosure can be affixed to packaging material or can be included as a package insert. While the instructions are typically written or printed materials they are not limited to such. Any medium capable of storing such instructions and communicating them to an end user is contemplated by this disclosure. Such media include, but are not limited to, electronic storage media (e.g., magnetic discs, tapes, cartridges, chips), optical media (e.g., CD ROM), and the like. As used herein, the term "instructions" can include the address of an internet site that provides the instructions.

D. ADAPTATIONS OF THE METHODS OF THE PRESENT DISCLOSURE

[0178] The present disclosure is for example applicable to the jointly owned commercial Abbott Point of Care (i-STATTM) electrochemical immunoassay system which performs sandwich immunoassays for several cardiac markers, including TnI, CKMB and BNP. Immunosensors and ways of operating them in single-use test devices are described in jointly owned Publication Nos. US 20030170881, US 20040018577, US 20050054078, and US 20060160164, each of which is incorporated herein by reference. Additional background on the manufacture of electrochemical and other types of immunosensors is found in jointly owned U.S. Pat. No. 5,063,081 which is also incorporated by reference.


[0179] By way of example, not of limitation, examples of the present invention shall now be given.

Example 1

Detection Antibody Conjugates

[0180] General Conjugation Procedure: Detection antibody was dissolved in a conjugation buffer (100 mM sodium phosphate, 150 mM NaCl, pH 8.0) to give a concentration of 1-10 mg/mL (6.25-62.5 μ M). Acridinium, 9-[[[4-(2,5-dioxo-1-pyrrolidinyl)oxy]-4-oxobutyl]][(4-methylphenyl)sulfonyl] amino]carbonyl]-10-(3-sulfopropyl)-, inner salt, 2 (Adamczyk, M.; Chen, Y.-Y.; Mattingly, P. G.; Pan, Y. *J. Org. Chem.*

1998, 63, 5636-5639) labeling reagent was prepared in N,N-dimethylformamide (DMF) at a concentration of 1-50 mM, as shown in formula 2 below:

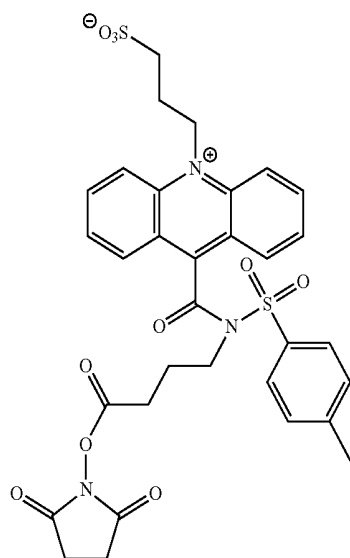

[0181] The selected antibody was treated with the acridinium-labeling reagent in a molar excess of 1-35 fold for 3-14 h at ambient temperature in the dark. Afterwards, the acridinium-9-carboxamide-antibody conjugate solution was dialyzed at ambient temperature over 20 hours using a 10 kilodalton molecular weight cutoff membrane against three volumes (1000× conjugate solution volume) of a dialysis buffer consisting of 10 mM phosphate buffered saline (PBS) containing 0.1% CHAPS (3-[(3-cholamidopropyl)dimethylammonio]-1-propanesulfonate).

[0182] The acridinium-9-carboxamide-antibody conjugate was analyzed by UV absorbance at 280/369 nm to determine the incorporation ratio (IR) of the acridinium-9-carboxamide label to the protein calculated according to the formula:

$$IR = A_{369} / \epsilon_{369} / ([A_{280} - (A_{369}/4.1)] / \epsilon_{280})$$

where:

[0183] A₂₈₀ and A₃₆₉ are absorbance values obtained from the UV-visible spectrum of the conjugate;

[0184] 4.1 is the ~A₃₆₉/A₂₈₀ ratio for an acridinium-9-carboxamide label;

[0185] ϵ_{280} is the extinction coefficient for an antibody at 280 nm (i.e., for IgG mAb $\epsilon_{280} = 210,000 \text{ M}^{-1} \text{ cm}^{-1}$); and

[0186] ϵ_{369} is the extinction coefficient for an acridinium-9-carboxamide label at 369 nm.

[0187] The average incorporation ratio for pooled fractions can range from 0.4-0.8× the molar excess of the acridinium-9-carboxamide labeling reagent used.

[0188] a) Murine anti-cardiac troponin-T 7G7 (Biodesign International/Meridian Life Sciences, Saco, Me.; cat no H86429M) mapped to epitope cTnT₆₀₋₇₀ was dialyzed against PBS to give a solution concentration of 0.35 mg/mL. After conjugation the calculated IR was 3.1.

[0189] b) Murine anti-cardiac troponin-T 7F4 (Fitzgerald Ind Intl, Concord, Mass., cat no. 10R-T127C) mapped to epitope cTnT₆₁₋₇₀ was dialyzed against PBS to give a solution concentration of 0.469 mg/mL. After conjugation the calculated IR was 2.8.

[0190] c) Murine anti-cardiac troponin-T 1C11 (Fitzgerald Ind Intl, Concord, Mass., cat no. 10R-T127D) mapped to epitope cTnT cTnT₉₅₋₁₈₁ was dialyzed against PBS to give a solution concentration of 0.469 mg/mL. After conjugation the calculated IR was 2.8.

[0191] d) Murine anti-cardiac troponin-T M8020207 (Fitzgerald Ind Intl, Concord, Mass., cat no. 10R-T85D) mapped primarily to epitope cTnT cTnT₇₃₋₈₇ was dialyzed against PBS to give a solution concentration of 0.413 mg/mL. After conjugation the calculated IR was 4.1.

Example 2

Capture Antibodies on Magnetic Microparticles

[0192] Carboxy paramagnetic microparticles (5% solids, nominally 5 micron diameter, Polymer Labs, Varian, Inc. Amherst, Mass.) were diluted to a concentration of 1% solids in 2-(N-morpholino)ethanesulfonic acid buffer (MES, 2 mL, pH 6.2, 50 mM) then washed with MES buffer (3×, 2 mL), and finally, resuspended in MES (2 mL). The particles were activated by mixing with 1-ethyl-3-[3-dimethylaminopropyl] carbodiimide hydrochloride (20 μL of 11 mg/1.129 mL in water) for 20 min, then washed (MES, 2 mL) and re-suspended in MES (2 mL). Murine anti-cardiac troponin-T 1C11 (Fitzgerald Ind Intl, Concord, Mass., cat no. 10R-T127D) was added to the suspension at 60 $\mu\text{g}/\text{mL}$. After mixing for 60 min the antigen coated particles were magnetically sequestered, and the antigen solution was replaced with a blocking solution consisting of 1% BSA in PBS (2 mL). After mixing for 30 min, the particles were washed with 1% BSA in PBS (3×, 2 mL) and finally, resuspended in 1% BSA in PBS (2 mL) and adjusted to a final concentration of 1% solids.

[0193] Microparticles were similarly prepared with the following murine anti-cardiac troponin-T antibodies: 7G7 (Biodesign International/Meridian Life Sciences, Saco, Me.; cat no H86429M); 7F4 (Fitzgerald Ind Intl, Concord, Mass., cat no. 10R-T127C); and M8020207 (Fitzgerald Ind Intl, Concord, Mass., cat no. 10R-T85D).

Example 3

Chemiluminescent Immunoassay Dose-Response for Combinations of Capture and Detection Antibodies

[0194] A working suspension of each capture antibody microparticles prepared in Example 2 was prepared by dilution of the stock suspension to 0.05% solids in MES buffer (20 mM, pH 6.6) containing sucrose (13.6%) and antimicrobial agents. A working solution of each detection antibody conjugate was prepared by dilution of the stock solution to 10 ng/mL. Cardiac troponin-T (Biospecific, cat no. J34510359) standard solutions were prepared at 0, 0.25, 0.5, 1.0 and 2.0 $\mu\text{g}/\text{mL}$.

[0195] The assays were carried out on an ARCHITECT® i2000 instrument (Abbott Laboratories, Abbott Park, Ill.). Briefly, the cardiac troponin-T standard solution (10 μL) was diluted with ARCHITECT® PreIncubation Diluent (50 μL) and the capture antibody microparticles (50 μL) and incubated in the instrument reaction vessel. Following incubation, the microparticles were magnetically sequestered and washed with ARCHITECT® wash buffer. The detection antibody solution (50 μL) was added, the suspension incubated, and then the microparticles were washed again. ARCHITECT® pre-trigger solution containing hydrogen peroxide and ARCHITECT® trigger solution containing sodium hydroxide were then sequentially added and the chemiluminescent signal (relative light units, RLU) were recorded. The dose-response curves for combinations of capture and detection antibodies are shown in Table 1 and graphically in FIG. 1.

TABLE 1

Troponin-T (µg/mL)	Detection conjugate/capture antibody (RLU)								
	7G7/ 7F4	7G7/ M8020207	7G7/ 1C11	7F4/ 7G7	7F4/ M8020207	7F4/ 1C11	M8020207/ 7G7	M8020207/ 7F4	M8020207/ 1C11
2	46829	305420	310518	6870	184343	185886	137713	100426	202062
1	29877	250755	238464	1469	136026	127325	106585	71224	157435
0.5	17246	163605	148894	618	82486	63012	70107	45245	105484
0.25	9081	96153	79374	452	38363	26439	42508	25611	66447
0	333	338	317	269	297	256	367	379	368

Example 4

Epitope Mapping of Autoantibodies to Cardiac Troponin T

[0196] Antibodies were screened against a biotinylated peptide library (Table 2) covering the entire human cTnT amino acid sequence as shown in FIG. 2 (UniProtKB/Swiss-Prot P45379 (TNNT2_HUMAN), initiator methionine removed, 297 aa, SEQ ID NO: 96), each peptide length, 15 aa; overlap, 12 aa; PEPscreen®, Sigma-Genosys, The Woodlands, Tex.) on streptavidin-coated microplates (Reacti-Bind™, Streptavidin; Pierce, Rockford, Ill.).

[0197] Thus, the peptides (100 µL, 1200 pmol/mL) were arrayed on the microplate; the microplate was then sealed and incubated/mixed for 1 h at ambient temperature. The microplate was then washed with ARCHITECT® wash buffer and aspirated to dryness. Samples (500 µL) were diluted with 9.5 mL of AxSYM Troponin Preincubation diluent then arrayed (100 µL/well) to the microplates with the peptide library. The plates were sealed and incubated at 37° C., mixing at 28 rpm for 2 h. Afterwards the plates were washed with ARCHITECT® wash buffer and the response against each peptide was determined using chemiluminescent detection on a Berthold Mithras microplate reader (Berthold Technologies Inc, Oak Ridge, Tenn.). A mouse anti-human IgG acridinium labeled conjugate solution (100 µL) was added to each test well. After the conjugate was added to all test samples, the microplate was then sealed, placed on an orbital shaker at 28 rpm and incubated at 37° C. for 1 h. The conjugate solution was then removed and the wells of the microplate were washed with the ARCHITECT® Line Diluent (3x300 µL). The microplate was loaded into the instrument that had been equilibrated at 37° C. ARCHITECT® Pre-Trigger solution (100 µL) was dispensed to each well. After the pre-trigger solution was added, the plate was shaken for 72 s. Then the ARCHITECT® Trigger solution (100 µL) was dispensed to each well and chemiluminescent signal recorded for 2 s. FIG. 3 shows the frequency of reactive cardiac troponin-T epitopes found in human cardiac troponin-T autoantibodies.

TABLE 2

cTnT Antigen Peptide Library		
Peptide No. (SEQ ID NO.):	cTnT sequence	Sequence No.
1	SDIEEVVEEYEEEEQ	1-15
2	EEVVEEYEEEEQEBA	4-18

TABLE 2-continued

cTnT Antigen Peptide Library		
Peptide No. (SEQ ID NO.):	cTnT sequence	Sequence No.
3	VEEYEEEEQEAAVE	7-21
4	YEEEEQEAAVEEEEE	10-24
5	EEQEAAVEEEEDWR	13-27
6	EAAVEEEEDWREDE	16-30
7	AVEEEEDWREDEDEQ	19-33
8	EEEDWREDEDEQEEA	22-36
9	DWREDEDEQEAAEE	25-39
10	EDEDEQEAAEEDAE	28-42
11	DEQEAAEEDAEAEA	31-45
12	EEAAEEDAEAEAETE	34-48
13	AEEEDAEAEAETEETR	37-51
14	DAAEAETEETRAEE	40-54
15	AEAETEETRAEEDDE	43-57
16	ETEETRAEEDDEEEEE	46-60
17	ETRAEEDDEEEEAKE	49-63
18	AEEDEEEEAKEAED	52-66
19	DEEEEAKEAEDGPM	55-69
20	EEEAKEAEDGPMEEES	58-72
21	AKEAEDGPMEEKPK	61-75
22	AEDGPMEEKPKPRRS	64-78
23	GPMEESKPKPRSFMP	67-81
24	EESKPKPRSFMPNLV	70-84
25	KPKPRSFMPNLVPPK	73-87
26	PRSFMPNLVPPKIPD	76-90
27	FMPNLVPPKIPDGER	79-93
28	NLVPPKIPDGERVDF	82-96
29	PPKIPDGERVDFDDI	85-99

TABLE 2-continued

cTnT Antigen Peptide Library		
Peptide No. (SEQ ID NO.):	cTnT sequence	Sequence No.
30	IPDGERVDFDDIHRK	88-102
31	GERVDFDDIHRKRME	91-105
32	VDFDDIHRKRMEKDL	94-108
33	DDIHRKRMEKDLNEL	97-111
34	HRKRMEKDLNELQAL	100-114
35	RMEKDLNELQALIEA	103-117
36	KDLNELQALIEAHFE	106-120
37	NELQALIEAHFENRK	109-123
38	QALIEAHFENRKKKEE	112-126
39	IEAHFENRKKKEEEL	115-129
40	HFENRKKKEEELVSL	118-132
41	NRKKEEELVSLKDR	121-135
42	KEEELVSLKDRIER	124-138
43	EELVSLKDRIERRRA	127-141
44	VSLKDRIERRRAERA	130-144
45	KDRIERRRAERAQQ	133-147
46	IERRRAERAQQQRIR	136-150
47	RRAERAQQQRIRNER	139-153
48	ERAQQQRIRNEREKE	142-156
49	EQQRIRNEREKERQN	145-159
50	RIRNEREKERQNRLA	148-162
51	NEREKERQNRLAEBER	151-165
52	EKERQNRLAEBERARR	154-168
53	RQNRLAEBERARREEE	157-171
54	RLAEBERARREEEENR	160-174
55	EERARREEEENRRKA	163-177
56	ARREEEENRRKAEDE	166-180
57	EEEENRRKAEDEARK	169-183
58	ENRRKAEDEARKKKA	172-186
59	RKAEDEARKKKALSN	175-189
60	EDEARKKKALSNMMH	178-192
61	ARKKKALSNMMHFGG	181-195
62	KKALSNMMHFGGYIQ	184-198
63	LSNMMHFGGYIQQA	187-201
64	MMHFGGYIQQAQTE	190-204

TABLE 2-continued

cTnT Antigen Peptide Library		
Peptide No. (SEQ ID NO.):	cTnT sequence	Sequence No.
65	FGGYIQQAQTERKS	193-207
66	YIQQAQTERKSGKR	196-210
67	KQAQTERKSGKRQTE	199-213
68	QTERKSGKRQTEREK	202-216
69	RKSGKRQTEREKKKK	205-219
70	GKRQTEREKKKKILA	208-222
71	QTEREKKKKILAERR	211-225
72	REKKKILAERRKVL	214-228
73	KKKILAERRKVLAI	217-231
74	ILAERRKVLAIIDL	220-234
75	ERRKVLAIIDLNEDQ	223-237
76	KVLAIIDLNLNEDQL	226-240
77	AIDLNLNEDQLREK	229-243
78	HLNEDQLREKAKEL	232-246
79	EDQLREKAKELWQ	235-249
80	LREKAKELWQSIYN	238-252
81	KAKELWQSIYNLEA	241-255
82	ELWQSIYNLEAEK	244-258
83	QSIYNLEAEKFDLQ	247-261
84	YNLEAEKFDLQEK	250-264
85	EAEKFDLQEKFKQ	253-267
86	KFDLQEKFKQKYEI	256-270
87	LQEKFKQKYEINVL	259-273
88	KFKQKYEINVLRR	262-276
89	QKYEINVLRRIND	265-279
90	YEINVLRRINDNQ	268-282
91	NVLRRINDNQKVS	271-285
92	RNRINDNQKVS	274-288
93	INDNQKVS	277-291
94	NQKVS	280-294
95	VSKTRGKAKVTGR	283-297

Example 5

Epitope Mapping of Monoclonal Antibodies to Cardiac Troponin-T

[0198] Murine anti-cardiac troponin-T M8020207 acridinium-9-carboxamide conjugate from Example 1 was

screened against a biotinylated peptide library (Table 2, Example 4). The conjugate was diluted to 100 ng/mL then the conjugate solution (100 μ L) was added to each test well. After the conjugate was added, the microplate was then sealed, placed on an orbital shaker at 28 rpm and incubated at 37° C. for 1 h. The conjugate solution was then removed and the wells of the microplate were washed with the ARCHITECT® Line Diluent (3 \times 300 μ L). The microplate was loaded into the instrument that had been equilibrated at 37° C. ARCHITECT® Pre-Trigger solution (100 μ L) was dispensed to each well. After the pre-trigger solution was added, the plate was shaken for 72 s. Then the ARCHITECT® Trigger solution (100 μ L) was dispensed to each well and chemiluminescent signal recorded for 2 s.

[0199] As shown in FIG. 4, the primary response was to peptide 25 corresponding to cTnT₇₃₋₈₇.

[0200] Murine anti-cardiac troponin-T 1C11 from Example 1 was screened against a biotinylated peptide library (Table 2, Example 4). The antibody was diluted to 100 ng/mL, then 100 μ L was added to each test well. The plate was sealed and incubated at 37° C., mixing at 28 rpm for 2 h. Afterwards the plates were washed with ARCHITECT® wash buffer. A goat anti-mouse IgG acridinium labeled conjugate solution (100 μ L) was added to each test well. After the conjugate was added to all test samples, the microplate was then sealed, placed on an orbital shaker at 28 rpm and incubated at 37° C. for 1 h. The conjugate solution was then removed and the wells of the microplate were washed with the ARCHITECT® Line Diluent (3 \times 300 μ L). The microplate was loaded into the instrument that had been equilibrated at 37° C. ARCHITECT® Pre-Trigger solution (100 μ L) was dispensed to each well. After the pre-trigger solution was added, the plate was shaken for 72 s. Then the ARCHITECT® Trigger solution (100 μ L) was dispensed to each well and chemiluminescent signal recorded for 2 s. As shown in FIG. 5, the primary epitopic response was to peptide 61 corresponding to cTnT₁₈₁₋₁₉₅.

Example 6

Standard Curve for Cardiac Troponin-T

[0201] Murine anti-cardiac troponin-T M8020207 coated microparticles from Example 2 were diluted to 0.3% solids. Murine anti-cardiac troponin-T 7G7 acridinium-9-carboxamide conjugate from Example 1 was diluted to 30 ng/mL. Standard solutions were made from human cardiac troponin I-T-C complex (HyTest, Turku Finland, catalog no. 8T62) to give cTnT concentrations: 0, 7.0, 14.0, 42.0, and 279.0 pM. Three test samples were prepared by spiking hcTnTC into negative human plasma to give nominal cTnT concentrations of 0, 7.0 and 42 pM. The standard solutions and human plasma samples were analyzed on an ARCHITECT® i2000 as in Example 3. A point to point calibration curve was plotted (RLU vs cTnT concentration). The results are listed in Table 3.

TABLE 3

Magnetic microparticle cardiac troponin T assay results		
Sample	RLU	pM cTnT
Cal A	2,369	0
Cal B	15,275	7
Cal C	28,071	14
Cal D	81,462	42
Cal E	422,814	279
Negative plasma	2,074	#N/A
Spiked plasma @7 pM	13,788	6.18
Spiked plasma @42 pM	74,126	38.07

[0202] One skilled in the art would readily appreciate that the immunoassays described in the present disclosure are well adapted to carry out the objects and obtain the ends and advantages mentioned, as well as those inherent therein. The molecular complexes and the methods, procedures, treatments, molecules, specific compounds described herein are presently representative of preferred embodiments, are exemplary, and are not intended as limitations on the scope of the invention. It will be readily apparent to one skilled in the art that varying substitutions and modifications may be made to the present disclosure disclosed herein without departing from the scope and spirit of the invention.

[0203] All patents and publications mentioned in the specification are indicative of the levels of those skilled in the art to which the present disclosure pertains. All patents and publications are herein incorporated by reference to the same extent as if each individual publication was specifically and individually indicated to be incorporated by reference.

[0204] The present disclosure illustratively described herein suitably may be practiced in the absence of any element or elements, limitation or limitations which are not specifically disclosed herein. Thus, for example, in each instance herein any of the terms “comprising,” “consisting essentially of” and “consisting” of may be replaced with either of the other two terms. The terms and expressions which have been employed are used as terms of description and not of limitation, and there is no intention that in the use of such terms and expressions of excluding any equivalents of the features shown and described or portions thereof, but it is recognized that various modifications are possible within the scope of the present disclosure claimed. Thus, it should be understood that although the present disclosure has been specifically disclosed by preferred embodiments and optional features, modification and variation of the concepts herein disclosed may be resorted to by those skilled in the art, and that such modifications and variations are considered to be within the scope of this invention as defined by the appended claims.

SEQUENCE LISTING

<160> NUMBER OF SEQ ID NOS: 96

<210> SEQ ID NO 1

-continued

<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 1

Ser Asp Ile Glu Glu Val Val Glu Glu Tyr Glu Glu Glu Glu Gln
1 5 10 15

<210> SEQ ID NO 2
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 2

Glu Glu Val Val Glu Glu Tyr Glu Glu Glu Glu Gln Glu Glu Ala
1 5 10 15

<210> SEQ ID NO 3
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 3

Val Glu Glu Tyr Glu Glu Glu Glu Gln Glu Glu Ala Ala Val Glu
1 5 10 15

<210> SEQ ID NO 4
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 4

Tyr Glu Glu Glu Glu Gln Glu Glu Ala Ala Val Glu Glu Glu Glu
1 5 10 15

<210> SEQ ID NO 5
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 5

Glu Glu Gln Glu Glu Ala Ala Val Glu Glu Glu Glu Asp Trp Arg
1 5 10 15

<210> SEQ ID NO 6
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 6

Glu Glu Ala Ala Val Glu Glu Glu Glu Asp Trp Arg Glu Asp Glu
1 5 10 15

<210> SEQ ID NO 7
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 7

Ala Val Glu Glu Glu Glu Asp Trp Arg Glu Asp Glu Asp Glu Gln
1 5 10 15

-continued

<210> SEQ ID NO 8
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 8

Glu Glu Glu Asp Trp Arg Glu Asp Glu Asp Glu Gln Glu Glu Ala
1 5 10 15

<210> SEQ ID NO 9
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 9

Asp Trp Arg Glu Asp Glu Asp Glu Gln Glu Glu Ala Ala Glu Glu
1 5 10 15

<210> SEQ ID NO 10
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 10

Glu Asp Glu Asp Glu Gln Glu Glu Ala Ala Glu Glu Asp Ala Glu
1 5 10 15

<210> SEQ ID NO 11
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 11

Asp Glu Gln Glu Glu Ala Ala Glu Glu Asp Ala Glu Ala Glu Ala
1 5 10 15

<210> SEQ ID NO 12
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 12

Glu Glu Ala Ala Glu Glu Asp Ala Glu Ala Glu Ala Glu Thr Glu
1 5 10 15

<210> SEQ ID NO 13
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 13

Ala Glu Glu Asp Ala Glu Ala Glu Ala Glu Thr Glu Glu Thr Arg
1 5 10 15

<210> SEQ ID NO 14
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 14

Asp Ala Glu Ala Glu Ala Glu Thr Glu Glu Thr Arg Ala Glu Glu
1 5 10 15

-continued

<210> SEQ ID NO 15
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 15

Ala Glu Ala Glu Thr Glu Glu Thr Arg Ala Glu Glu Asp Glu Glu
1 5 10 15

<210> SEQ ID NO 16
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 16

Glu Thr Glu Glu Thr Arg Ala Glu Glu Asp Glu Glu Glu Glu Glu
1 5 10 15

<210> SEQ ID NO 17
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 17

Glu Thr Arg Ala Glu Glu Asp Glu Glu Glu Glu Glu Ala Lys Glu
1 5 10 15

<210> SEQ ID NO 18
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 18

Ala Glu Glu Asp Glu Glu Glu Glu Glu Ala Lys Glu Ala Glu Asp
1 5 10 15

<210> SEQ ID NO 19
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 19

Asp Glu Glu Glu Glu Glu Ala Lys Glu Ala Glu Asp Gly Pro Met
1 5 10 15

<210> SEQ ID NO 20
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 20

Glu Glu Glu Ala Lys Glu Ala Glu Asp Gly Pro Met Glu Glu Ser
1 5 10 15

<210> SEQ ID NO 21
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 21

Ala Lys Glu Ala Glu Asp Gly Pro Met Glu Glu Ser Lys Pro Lys
1 5 10 15

-continued

<210> SEQ ID NO 22

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 22

Ala Glu Asp Gly Pro Met Glu Glu Ser Lys Pro Lys Pro Arg Ser
1 5 10 15

<210> SEQ ID NO 23

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 23

Gly Pro Met Glu Glu Ser Lys Pro Lys Pro Arg Ser Phe Met Pro
1 5 10 15

<210> SEQ ID NO 24

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 24

Glu Glu Ser Lys Pro Lys Pro Arg Ser Phe Met Pro Asn Leu Val
1 5 10 15

<210> SEQ ID NO 25

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 25

Lys Pro Lys Pro Arg Ser Phe Met Pro Asn Leu Val Pro Pro Lys
1 5 10 15

<210> SEQ ID NO 26

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 26

Pro Arg Ser Phe Met Pro Asn Leu Val Pro Pro Lys Ile Pro Asp
1 5 10 15

<210> SEQ ID NO 27

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 27

Phe Met Pro Asn Leu Val Pro Pro Lys Ile Pro Asp Gly Glu Arg
1 5 10 15

<210> SEQ ID NO 28

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 28

Asn Leu Val Pro Pro Lys Ile Pro Asp Gly Glu Arg Val Asp Phe

-continued

1 5 10 15

<210> SEQ ID NO 29
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 29

Pro Pro Lys Ile Pro Asp Gly Glu Arg Val Asp Phe Asp Asp Ile
1 5 10 15

<210> SEQ ID NO 30
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 30

Ile Pro Asp Gly Glu Arg Val Asp Phe Asp Asp Ile His Arg Lys
1 5 10 15

<210> SEQ ID NO 31
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 31

Gly Glu Arg Val Asp Phe Asp Asp Ile His Arg Lys Arg Met Glu
1 5 10 15

<210> SEQ ID NO 32
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 32

Val Asp Phe Asp Asp Ile His Arg Lys Arg Met Glu Lys Asp Leu
1 5 10 15

<210> SEQ ID NO 33
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 33

Asp Asp Ile His Arg Lys Arg Met Glu Lys Asp Leu Asn Glu Leu
1 5 10 15

<210> SEQ ID NO 34
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 34

His Arg Lys Arg Met Glu Lys Asp Leu Asn Glu Leu Gln Ala Leu
1 5 10 15

<210> SEQ ID NO 35
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 35

-continued

Arg Met Glu Lys Asp Leu Asn Glu Leu Gln Ala Leu Ile Glu Ala
1 5 10 15

<210> SEQ ID NO 36
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 36

Lys Asp Leu Asn Glu Leu Gln Ala Leu Ile Glu Ala His Phe Glu
1 5 10 15

<210> SEQ ID NO 37
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 37

Asn Glu Leu Gln Ala Leu Ile Glu Ala His Phe Glu Asn Arg Lys
1 5 10 15

<210> SEQ ID NO 38
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 38

Gln Ala Leu Ile Glu Ala His Phe Glu Asn Arg Lys Lys Glu Glu
1 5 10 15

<210> SEQ ID NO 39
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 39

Ile Glu Ala His Phe Glu Asn Arg Lys Lys Glu Glu Glu Glu Leu
1 5 10 15

<210> SEQ ID NO 40
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 40

His Phe Glu Asn Arg Lys Lys Glu Glu Glu Glu Leu Val Ser Leu
1 5 10 15

<210> SEQ ID NO 41
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 41

Asn Arg Lys Lys Glu Glu Glu Glu Leu Val Ser Leu Lys Asp Arg
1 5 10 15

<210> SEQ ID NO 42
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 42

-continued

Lys Glu Glu Glu Glu Leu Val Ser Leu Lys Asp Arg Ile Glu Arg
1 5 10 15

<210> SEQ ID NO 43
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 43

Glu Glu Leu Val Ser Leu Lys Asp Arg Ile Glu Arg Arg Arg Ala
1 5 10 15

<210> SEQ ID NO 44
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 44

Val Ser Leu Lys Asp Arg Ile Glu Arg Arg Arg Ala Glu Arg Ala
1 5 10 15

<210> SEQ ID NO 45
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 45

Lys Asp Arg Ile Glu Arg Arg Arg Ala Glu Arg Ala Glu Gln Gln
1 5 10 15

<210> SEQ ID NO 46
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 46

Ile Glu Arg Arg Arg Ala Glu Arg Ala Glu Gln Gln Arg Ile Arg
1 5 10 15

<210> SEQ ID NO 47
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 47

Arg Arg Ala Glu Arg Ala Glu Gln Gln Arg Ile Arg Asn Glu Arg
1 5 10 15

<210> SEQ ID NO 48
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 48

Glu Arg Ala Glu Gln Gln Arg Ile Arg Asn Glu Arg Glu Lys Glu
1 5 10 15

<210> SEQ ID NO 49
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

-continued

<400> SEQUENCE: 49

Glu Gln Gln Arg Ile Arg Asn Glu Arg Glu Lys Glu Arg Gln Asn
1 5 10 15

<210> SEQ ID NO 50

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 50

Arg Ile Arg Asn Glu Arg Glu Lys Glu Arg Gln Asn Arg Leu Ala
1 5 10 15

<210> SEQ ID NO 51

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 51

Asn Glu Arg Glu Lys Glu Arg Gln Asn Arg Leu Ala Glu Glu Arg
1 5 10 15

<210> SEQ ID NO 52

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 52

Glu Lys Glu Arg Gln Asn Arg Leu Ala Glu Glu Arg Ala Arg Arg
1 5 10 15

<210> SEQ ID NO 53

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 53

Arg Gln Asn Arg Leu Ala Glu Glu Arg Ala Arg Arg Glu Glu Glu
1 5 10 15

<210> SEQ ID NO 54

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 54

Arg Leu Ala Glu Glu Arg Ala Arg Arg Glu Glu Glu Glu Asn Arg
1 5 10 15

<210> SEQ ID NO 55

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 55

Glu Glu Arg Ala Arg Arg Glu Glu Glu Glu Asn Arg Arg Lys Ala
1 5 10 15

<210> SEQ ID NO 56

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

-continued

<400> SEQUENCE: 56

Ala Arg Arg Glu Glu Glu Glu Asn Arg Arg Lys Ala Glu Asp Glu
1 5 10 15

<210> SEQ ID NO 57

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 57

Glu Glu Glu Glu Asn Arg Arg Lys Ala Glu Asp Glu Ala Arg Lys
1 5 10 15

<210> SEQ ID NO 58

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 58

Glu Asn Arg Arg Lys Ala Glu Asp Glu Ala Arg Lys Lys Lys Ala
1 5 10 15

<210> SEQ ID NO 59

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 59

Arg Lys Ala Glu Asp Glu Ala Arg Lys Lys Lys Ala Leu Ser Asn
1 5 10 15

<210> SEQ ID NO 60

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 60

Glu Asp Glu Ala Arg Lys Lys Lys Ala Leu Ser Asn Met Met His
1 5 10 15

<210> SEQ ID NO 61

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 61

Ala Arg Lys Lys Lys Ala Leu Ser Asn Met Met His Phe Gly Gly
1 5 10 15

<210> SEQ ID NO 62

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 62

Lys Lys Ala Leu Ser Asn Met Met His Phe Gly Gly Tyr Ile Gln
1 5 10 15

<210> SEQ ID NO 63

<211> LENGTH: 15

<212> TYPE: PRT

-continued

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 63

Leu Ser Asn Met Met His Phe Gly Gly Tyr Ile Gln Lys Gln Ala
1 5 10 15

<210> SEQ ID NO 64

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 64

Met Met His Phe Gly Gly Tyr Ile Gln Lys Gln Ala Gln Thr Glu
1 5 10 15

<210> SEQ ID NO 65

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 65

Phe Gly Gly Tyr Ile Gln Lys Gln Ala Gln Thr Glu Arg Lys Ser
1 5 10 15

<210> SEQ ID NO 66

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 66

Tyr Ile Gln Lys Gln Ala Gln Thr Glu Arg Lys Ser Gly Lys Arg
1 5 10 15

<210> SEQ ID NO 67

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 67

Lys Gln Ala Gln Thr Glu Arg Lys Ser Gly Lys Arg Gln Thr Glu
1 5 10 15

<210> SEQ ID NO 68

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 68

Gln Thr Glu Arg Lys Ser Gly Lys Arg Gln Thr Glu Arg Glu Lys
1 5 10 15

<210> SEQ ID NO 69

<211> LENGTH: 15

<212> TYPE: PRT

<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 69

Arg Lys Ser Gly Lys Arg Gln Thr Glu Arg Glu Lys Lys Lys Lys
1 5 10 15

<210> SEQ ID NO 70

<211> LENGTH: 15

-continued

<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 70
Gly Lys Arg Gln Thr Glu Arg Glu Lys Lys Lys Lys Ile Leu Ala
1 5 10 15

<210> SEQ ID NO 71
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 71

Gln Thr Glu Arg Glu Lys Lys Lys Lys Ile Leu Ala Glu Arg Arg
1 5 10 15

<210> SEQ ID NO 72
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 72

Arg Glu Lys Lys Lys Lys Ile Leu Ala Glu Arg Arg Lys Val Leu
1 5 10 15

<210> SEQ ID NO 73
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 73

Lys Lys Lys Ile Leu Ala Glu Arg Arg Lys Val Leu Ala Ile Asp
1 5 10 15

<210> SEQ ID NO 74
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 74

Ile Leu Ala Glu Arg Arg Lys Val Leu Ala Ile Asp His Leu Asn
1 5 10 15

<210> SEQ ID NO 75
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 75

Glu Arg Arg Lys Val Leu Ala Ile Asp His Leu Asn Glu Asp Gln
1 5 10 15

<210> SEQ ID NO 76
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens
<400> SEQUENCE: 76

Lys Val Leu Ala Ile Asp His Leu Asn Glu Asp Gln Leu Arg Glu
1 5 10 15

<210> SEQ ID NO 77

-continued

<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 77

Ala Ile Asp His Leu Asn Glu Asp Gln Leu Arg Glu Lys Ala Lys
1 5 10 15

<210> SEQ ID NO 78
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 78

His Leu Asn Glu Asp Gln Leu Arg Glu Lys Ala Lys Glu Leu Trp
1 5 10 15

<210> SEQ ID NO 79
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 79

Glu Asp Gln Leu Arg Glu Lys Ala Lys Glu Leu Trp Gln Ser Ile
1 5 10 15

<210> SEQ ID NO 80
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 80

Leu Arg Glu Lys Ala Lys Glu Leu Trp Gln Ser Ile Tyr Asn Leu
1 5 10 15

<210> SEQ ID NO 81
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 81

Lys Ala Lys Glu Leu Trp Gln Ser Ile Tyr Asn Leu Glu Ala Glu
1 5 10 15

<210> SEQ ID NO 82
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 82

Glu Leu Trp Gln Ser Ile Tyr Asn Leu Glu Ala Glu Lys Phe Asp
1 5 10 15

<210> SEQ ID NO 83
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 83

Gln Ser Ile Tyr Asn Leu Glu Ala Glu Lys Phe Asp Leu Gln Glu
1 5 10 15

-continued

<210> SEQ ID NO 84
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 84
Tyr Asn Leu Glu Ala Glu Lys Phe Asp Leu Gln Glu Lys Phe Lys
1 5 10 15

<210> SEQ ID NO 85
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 85
Glu Ala Glu Lys Phe Asp Leu Gln Glu Lys Phe Lys Gln Gln Lys
1 5 10 15

<210> SEQ ID NO 86
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 86
Lys Phe Asp Leu Gln Glu Lys Phe Lys Gln Gln Lys Tyr Glu Ile
1 5 10 15

<210> SEQ ID NO 87
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 87
Leu Gln Glu Lys Phe Lys Gln Gln Lys Tyr Glu Ile Asn Val Leu
1 5 10 15

<210> SEQ ID NO 88
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 88
Lys Phe Lys Gln Gln Lys Tyr Glu Ile Asn Val Leu Arg Asn Arg
1 5 10 15

<210> SEQ ID NO 89
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 89
Gln Gln Lys Tyr Glu Ile Asn Val Leu Arg Asn Arg Ile Asn Asp
1 5 10 15

<210> SEQ ID NO 90
<211> LENGTH: 15
<212> TYPE: PRT
<213> ORGANISM: Homo sapiens

<400> SEQUENCE: 90
Tyr Glu Ile Asn Val Leu Arg Asn Arg Ile Asn Asp Asn Gln Lys
1 5 10 15

-continued

Gln Glu Glu Ala Ala Glu Glu Asp Ala Glu Ala Glu Ala Glu Thr Glu
 35 40 45
 Glu Thr Arg Ala Glu Glu Asp Glu Glu Glu Glu Glu Ala Lys Glu Ala
 50 55 60
 Glu Asp Gly Pro Met Glu Glu Ser Lys Pro Lys Pro Arg Ser Phe Met
 65 70 75 80
 Pro Asn Leu Val Pro Pro Lys Ile Pro Asp Gly Glu Arg Val Asp Phe
 85 90 95
 Asp Asp Ile His Arg Lys Arg Met Glu Lys Asp Leu Asn Glu Leu Gln
 100 105 110
 Ala Leu Ile Glu Ala His Phe Glu Asn Arg Lys Lys Glu Glu Glu Glu
 115 120 125
 Leu Val Ser Leu Lys Asp Arg Ile Glu Arg Arg Arg Ala Glu Arg Ala
 130 135 140
 Glu Gln Gln Arg Ile Arg Asn Glu Arg Glu Lys Glu Arg Gln Asn Arg
 145 150 155 160
 Leu Ala Glu Glu Arg Ala Arg Arg Glu Glu Glu Glu Asn Arg Arg Lys
 165 170 175
 Ala Glu Asp Glu Ala Arg Lys Lys Lys Ala Leu Ser Asn Met Met His
 180 185 190
 Phe Gly Gly Tyr Ile Gln Lys Gln Ala Gln Thr Glu Arg Lys Ser Gly
 195 200 205
 Lys Arg Gln Thr Glu Arg Glu Lys Lys Lys Lys Ile Leu Ala Glu Arg
 210 215 220
 Arg Lys Val Leu Ala Ile Asp His Leu Asn Glu Asp Gln Leu Arg Glu
 225 230 235 240
 Lys Ala Lys Glu Leu Trp Gln Ser Ile Tyr Asn Leu Glu Ala Glu Lys
 245 250 255
 Phe Asp Leu Gln Glu Lys Phe Lys Gln Gln Lys Tyr Glu Ile Asn Val
 260 265 270
 Leu Arg Asn Arg Ile Asn Asp Asn Gln Lys Val Ser Lys Thr Arg Gly
 275 280 285
 Lys Ala Lys Val Thr Gly Arg Trp Lys
 290 295

What is claimed is:

1. An immunoassay for quantifying an amount of cardiac troponin-T (cTnT) in a test sample, the immunoassay comprising the steps of:

- a) contacting a test sample suspected of containing cTnT with n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody: cTnT complex (C₁)(C₂) . . . (C_n)(cTnT), wherein n is an integer from 1 to 10; and
- b) contacting said mixture comprising a n-capture antibody-cTnT epitope complex (C₁)(C₂) . . . (C_n)(cTnT) with n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody: n-capture antibody: cTnT measurable assembly (D₁)(D₂) . . . (D_{n'})(C₁)(C₂) . . . (C_n)(cTnT); and

wherein n' and n are independently an integer from 1 to 10, and antibodies C and D bind to (n+n') different epitopes of cTnT.

2. The immunoassay of claim 1, wherein, an optical, electrical, or change-of-state signal of the measurable assembly is measured.

3. The immunoassay of claim 1 or 2, wherein the detection antibodies are conjugated to a detectable label, wherein the detectable label is an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

4. The immunoassay of claim 1 or 2, wherein the capture antibodies, the detection antibodies or capture and detection antibodies comprise humanized antibodies.

5. The immunoassay of claim 1 or 2, wherein the detection antibodies comprise humanized antibodies complexed with an anti-human IgG antibody.

6. The immunoassay of claim 5, wherein said anti-human IgG antibody is conjugated to a detectable label, wherein the detectable label is an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

7. The immunoassay of claim 2, wherein the optical signal is measured as a cTnT concentration dependent change in chemiluminescence, fluorescence, phosphorescence, electrochemiluminescence, ultraviolet absorption, visible absorption, infrared absorption, refraction, surface plasmon resonance.

8. The immunoassay of claim 2, wherein the electrical signal is measured as a troponin-T concentration dependent change in current, resistance, potential, mass to charge ratio, or ion count.

9. The immunoassay of claim 2, wherein the change-of-state signal is measured as a troponin-T concentration dependent change in size, solubility, mass, or resonance.

10. The immunoassay of claim 1 or 2, wherein the capture antibodies are immobilized on a solid phase.

11. The immunoassay of claim 10, wherein the solid phase is selected from the group consisting of a magnetic particle, bead, test tube, microtiter plate, cuvette, membrane, a scaffolding molecule, quartz crystal, film, filter paper, disc and chip.

12. An immunoassay for quantifying an amount of cardiac troponin-T (cTnT) in a test sample, the immunoassay comprising the steps of:

- contacting a test sample suspected of containing cTnT with n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody: cTnT complex (C₁)(C₂) . . . (C_n)(cTnT), wherein n is an integer from 1 to 10;
- contacting said mixture comprising a n-capture antibody-cTnT epitope complex (C₁)(C₂) . . . (C_n)(cTnT) with n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody: n-capture antibody: cTnT measurable assembly (D₁)(D₂) . . . (D_{n'})(C₁)(C₂) . . . (C_n)(cTnT), wherein the detection antibodies D are labeled with a detectable label comprising at least one acridinium compound, n' and n are independently an integer from 1 to 10, and antibodies C and D bind to (n+n') different epitopes of cTnT;
- generating or providing a source of hydrogen peroxide to the mixture of step (b);
- adding a basic solution to the mixture of step (c) to generate a light signal;
- measuring the light signal generated by or emitted in step (d); and
- quantifying the amount of troponin-T in the test sample based on the measurement in step (e).


13. The immunoassay of claim 12, wherein the capture antibodies, the detection antibodies or capture and detection antibodies comprise humanized antibodies.

14. The immunoassay of claim 12, wherein the detection antibodies comprise humanized antibodies complexed with an anti-human IgG antibody.

15. The immunoassay of claim 14, wherein said anti-human IgG antibody is conjugated to the detectable label comprising at least one acridinium compound.


16. The immunoassay of claim 12, wherein the test sample is whole blood, serum, plasma.

17. The immunoassay of claim 12, wherein the acridinium compound is an acridinium-9-carboxamide having a structure according to formula I:

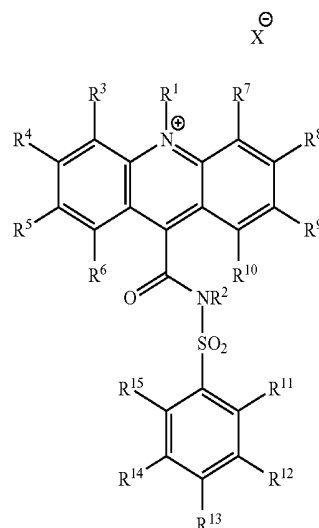

wherein R¹ and R² are each independently selected from the group consisting of: alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl, and wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and optionally, if present, X[⊖] is an anion.

18. The immunoassay of claim 12, wherein the acridinium compound is an acridinium-9-carboxylate aryl ester having a structure according to formula II:

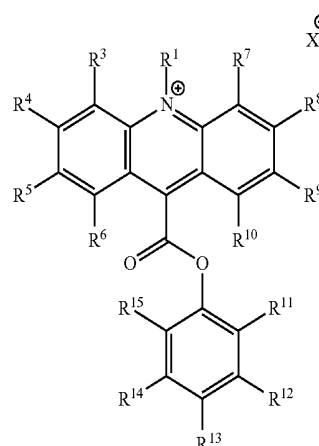

wherein R¹ is an alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and wherein R³ through R¹⁵ are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and optionally, if present, X[⊖] is an anion.

19. The immunoassay of claim 12, wherein the capture antibodies are immobilized on a solid phase.

20. The immunoassay of claim 19, wherein the solid phase is selected from the group consisting of a magnetic particle, bead, test tube, microtiter plate, cuvette, membrane, a scaffolding molecule, quartz crystal, film, filter paper, disc and chip.

21. The immunoassay of claim 12, wherein the capture antibodies are selected from the group consisting of a polyclonal antibody, a monoclonal antibody, a chimeric antibody, a human antibody, and an affinity matured antibody.

22. The immunoassay of claim 12, wherein the detection antibodies are selected from the group consisting of a polyclonal antibody, a monoclonal antibody, a chimeric antibody, a human antibody, and an affinity matured antibody.

23. The immunoassay of claim 12, wherein the hydrogen peroxide is provided by adding a buffer or a solution containing hydrogen peroxide.

24. The immunoassay of claim 12, wherein the hydrogen peroxide is generated by adding a hydrogen peroxide generating enzyme to the test sample.

25. The immunoassay of claim 24, wherein the hydrogen peroxide generating enzyme is selected from the group consisting of: (R)-6-hydroxynicotine oxidase, (S)-2-hydroxy acid oxidase, (S)-6-hydroxynicotine oxidase, 3-aci-nitropropanoate oxidase, 3-hydroxyanthranilate oxidase, 4-hydroxy-mandelate oxidase, 6-hydroxynicotinate dehydrogenase, abscisic-aldehyde oxidase, acyl-CoA oxidase, alcohol oxidase, aldehyde oxidase, amine oxidase, amine oxidase (copper-containing), amine oxidase (flavin-containing), aryl-alcohol oxidase, aryl-aldehyde oxidase, catechol oxidase, cholesterol oxidase, choline oxidase, columbamine oxidase, cyclohexylamine oxidase, cytochrome c oxidase, D-amino acid oxidase, D-arabinono-1,4-lactone oxidase, D-arabinono-1,4-lactone oxidase, D-aspartate oxidase, D-glutamate oxidase, D-glutamate(D-aspartate) oxidase, dihydrobenzophenanthridine oxidase, dihydroorotate oxidase, dihydrouracil oxidase, dimethylglycine oxidase, D-mannitol oxidase, ecdysone oxidase, ethanolamine oxidase, galactose oxidase, glucose oxidase, glutathione oxidase, glycerol-3-phosphate oxidase, glycine oxidase, glyoxylate oxidase, hexose oxidase, hydroxyphytanate oxidase, indole-3-acetaldehyde oxidase, lactic acid oxidase, L-amino acid oxidase, L-aspartate oxidase, L-galactonolactone oxidase, L-glutamate oxidase, L-gulonolactone oxidase, L-lysine 6-oxidase, L-lysine oxidase, long-chain-alcohol oxidase, L-pipecolate oxidase, L-sorbose oxidase, malate oxidase, methanethiol oxidase, monoamino acid oxidase, N6-methyl-lysine oxidase, N-acylhexosamine oxidase, NAD (P)H oxidase, nitroalkane oxidase, N-methyl-L-amino acid oxidase, nucleoside oxidase, oxalate oxidase, polyamine oxidase, polyphenol oxidase, polyvinyl-alcohol oxidase, prenyl-cysteine oxidase, protein-lysine 6-oxidase, putrescine oxidase, pyranose oxidase, pyridoxal 5'-phosphate synthase, pyridoxine 4-oxidase, pyrroloquinoline-quinone synthase, pyruvate oxidase, pyruvate oxidase (CoA-acetylating), reticuline oxidase, retinal oxidase, rifamycin-B oxidase, sarcosine oxidase, secondary-alcohol oxidase, sulfite oxidase, superoxide dismutase, superoxide reductase, tetrahydroberberine oxidase, thiamine oxidase, tryptophan α,β -oxidase, urate oxidase (uricase, uric acid oxidase), vanillyl-alcohol oxidase, xanthine oxidase, xylitol oxidase and combinations thereof.

26. The immunoassay of claim 12, wherein the basic solution is a solution having a pH of at least about 10.

27. The immunoassay of claim 12, further comprising the step of quantifying the amount of the troponin-T in the test sample by relating the amount of light signal in step (e) to the amount of troponin-T in the test sample either by use of a standard curve for cTnT or by comparison to a reference standard.

28. The immunoassay of claim 27, comprising comparison to a reference standard comprising an anti-idiotypic antibody.

29. The immunoassay of claim 27, comprising comparison to a reference standard comprising a derivatized troponin-T.

30. The immunoassay of claim 29, wherein the derivatized troponin-T comprises troponin-T derivatized with a polyethylene glycol.

31. The immunoassay of claim 12, wherein the immunoassay is adapted for use in an automated system or semi-automated system.

32. A kit for quantifying the amount of troponin-T in a test sample, the kit comprising: n capture antibodies (C) that bind to at least n epitopes on cTnT to form a n-capture antibody: cTnT complex (C₁)(C₂) . . . (C_n)(cTnT), wherein n is an integer from 1 to 10; n' detection antibodies (D) that bind to n' epitopes on cTnT to form a n'-detection antibody: n-capture antibody: cTnT measurable assembly (D₁)(D₂) . . . (D_{n'})(C₁)(C₂) . . . (C_n)(cTnT), wherein n' and n are independently an integer from 1 to 10; and wherein antibodies C and D bind to (n+n') different epitopes of cTnT; and instructions for quantifying the amount of cTnT in the test sample.

33. The kit of claim 32, wherein the capture antibodies are immobilized on a solid phase.


34. The kit of claim 33, wherein the solid phase is selected from the group consisting of a magnetic particle, a bead, a test tube, a microtiter plate, a cuvette, a membrane, a scaffolding molecule, a quartz crystal, a film, a filter paper, a disc and a chip.

35. The kit of claim 32, further comprising a detectable label conjugated to the detection antibodies.

36. The kit of claim 35, wherein the detectable label is an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

37. The kit of claim 35, wherein the detectable label is an acridinium compound.


38. The kit of claim 37, wherein the acridinium compound is an acridinium-9-carboxamide having a structure according to formula I:

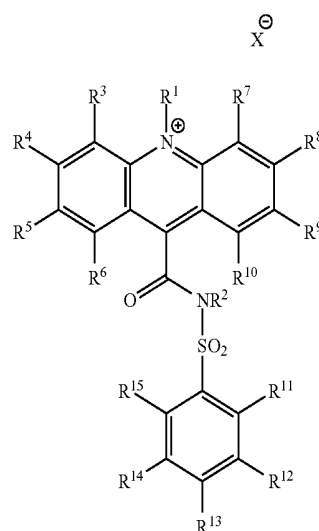

I

wherein R^1 and R^2 are each independently selected from the group consisting of: alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl, and wherein R^3 through R^{15} are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and optionally, if present, X^\ominus is an anion.

39. The kit of claim 37, wherein the acridinium compound is an acridinium-9-carboxylate aryl ester having a structure according to formula II:

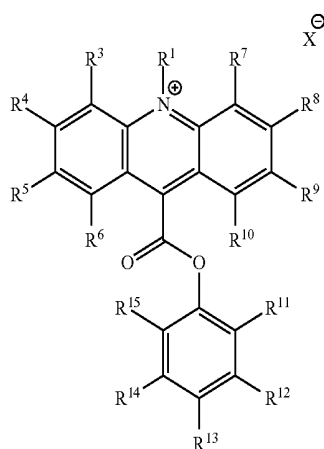

wherein R^1 is an alkyl, alkenyl, alkynyl, aryl or aralkyl, sulfoalkyl, carboxyalkyl and oxoalkyl; and wherein R^3 through R^{15} are each independently selected from the group consisting of: hydrogen, alkyl, alkenyl, alkynyl, aryl or aralkyl, amino, amido, acyl, alkoxy, hydroxyl, carboxyl, halogen, halide, nitro, cyano, sulfo, sulfoalkyl, carboxyalkyl and oxoalkyl; and optionally, if present, X^\ominus is an anion.

40. The kit of claim 37, further comprising a basic solution.

41. The kit of claim 40, wherein the basic solution is a solution having a pH of at least about 10.

42. The kit of claim 37, further comprising a hydrogen peroxide source.

43. The kit of claim 42, wherein the hydrogen peroxide source comprises a buffer or a solution containing hydrogen peroxide.

44. The kit of claim 42, wherein the hydrogen peroxide source comprises a hydrogen peroxide generating enzyme.

45. The kit of claim 44, wherein the hydrogen peroxide generating enzyme is selected from the group consisting of: (R)-6-hydroxynicotine oxidase, (S)-2-hydroxy acid oxidase, (S)-6-hydroxynicotine oxidase, 3-aci-nitropropanoate oxidase, 3-hydroxyanthranilate oxidase, 4-hydroxymandelate oxidase, 6-hydroxynicotinate dehydrogenase, abscisic-alde-

hyde oxidase, acyl-CoA oxidase, alcohol oxidase, aldehyde oxidase, amine oxidase, amine oxidase (copper-containing), amine oxidase (flavin-containing), aryl-alcohol oxidase, aryl-aldehyde oxidase, catechol oxidase, cholesterol oxidase, choline oxidase, columbamine oxidase, cyclohexylamine oxidase, cytochrome c oxidase, D-amino-acid oxidase, D-arabinono-1,4-lactone oxidase, D-arabinono-1,4-lactone oxidase, D-aspartate oxidase, D-glutamate oxidase, D-glutamate(D-aspartate)oxidase, dihydrobenzophenanthridine oxidase, dihydroorotate oxidase, dihydrouracil oxidase, dimethylglycine oxidase, D-mannitol oxidase, ecdysone oxidase, ethanolamine oxidase, galactose oxidase, glucose oxidase, glutathione oxidase, glycerol-3-phosphate oxidase, glycine oxidase, glyoxylate oxidase, hexose oxidase, hydroxyphytanate oxidase, indole-3-acetaldehyde oxidase, lactic acid oxidase, L-amino-acid oxidase, L-aspartate oxidase, L-galactonolactone oxidase, L-glutamate oxidase, L-gulonolactone oxidase, L-lysine 6-oxidase, L-lysine oxidase, long-chain-alcohol oxidase, L-pipecolate oxidase, L-sorbose oxidase, malate oxidase, methanethiol oxidase, monoamino acid oxidase, N6-methyl-lysine oxidase, N-acyl-hexosamine oxidase, NAD(P)H oxidase, nitroalkane oxidase, N-methyl-L-amino-acid oxidase, nucleoside oxidase, oxalate oxidase, polyamine oxidase, polyphenol oxidase, polyvinyl-alcohol oxidase, prenylcysteine oxidase, protein-lysine 6-oxidase, putrescine oxidase, pyranose oxidase, pyridoxal 5'-phosphate synthase, pyridoxine 4-oxidase, pyrroloquinoline-quinone synthase, pyruvate oxidase, pyruvate oxidase (CoA-acetylating), reticuline oxidase, retinal oxidase, rifamycin-B oxidase, sarcosine oxidase, secondary-alcohol oxidase, sulfite oxidase, superoxide dismutase, superoxide reductase, tetrahydroberberine oxidase, thiamine oxidase, tryptophan α,β -oxidase, urate oxidase (uricase, uric acid oxidase), vanillyl-alcohol oxidase, xanthine oxidase, xylitol oxidase and combinations thereof.

46. The kit of claim 32, wherein the capture antibodies, the detection antibodies or the capture and detection antibodies comprise humanized antibodies.

47. The kit of claim 32, wherein the detection antibodies comprise humanized antibodies complexed with an anti-human IgG antibody.

48. The kit of claim 47, wherein said anti-human IgG antibody is conjugated to a detectable label, wherein the detectable label is an enzyme, oligonucleotide, nanoparticle chemiluminophore, fluorophore, fluorescence quencher, chemiluminescence quencher, or biotin.

49. The kit of claim 32, further comprising a cTnT reference standard.

50. The kit of claim 49, wherein the cTnT reference standard comprises an anti-idiotypic antibody.

51. The kit of claim 49, wherein the cTnT reference standard comprises a derivatized cTnT.

52. The kit of claim 51, wherein the derivatized cTnT comprises cTnT derivatized with a polyethylene glycol.

* * * * *

专利名称(译)	CARDIAC TROPONIN-T (cTnT) 的分析		
公开(公告)号	US20110129818A1	公开(公告)日	2011-06-02
申请号	US12/629736	申请日	2009-12-02
[标]申请(专利权)人(译)	雅培公司		
申请(专利权)人(译)	亚培		
当前申请(专利权)人(译)	亚培		
[标]发明人	ADAMCZYK MACIEJ BRASHEAR JEFFREY R MATTINGLY PHILLIP G		
发明人	ADAMCZYK, MACIEJ BRASHEAR, JEFFREY R. MATTINGLY, PHILLIP G.		
IPC分类号	C12Q1/68 G01N33/53		
CPC分类号	G01N33/6893 G01N2800/324 G01N2800/32 G01N2333/4712		
其他公开文献	US8835120		
外部链接	Espacenet USPTO		

摘要(译)

本公开描述了免疫测定用于检测测试样品中心脏肌钙蛋白T (cTnT) 的，并且特别是免疫测定和试剂盒用于怀疑含有可与肌钙蛋白T，的干扰测定的物质的测试样品中检测的cTnT如异嗜性的内源性抗体和cTnT的自身抗体。该方法使用一种以上的捕获相抗体和一种以上的检测抗体来提高特异性，并提供人源化免疫试剂用于克服嗜异性抗体干扰的用途。

